


# CONSIDERING XENON?

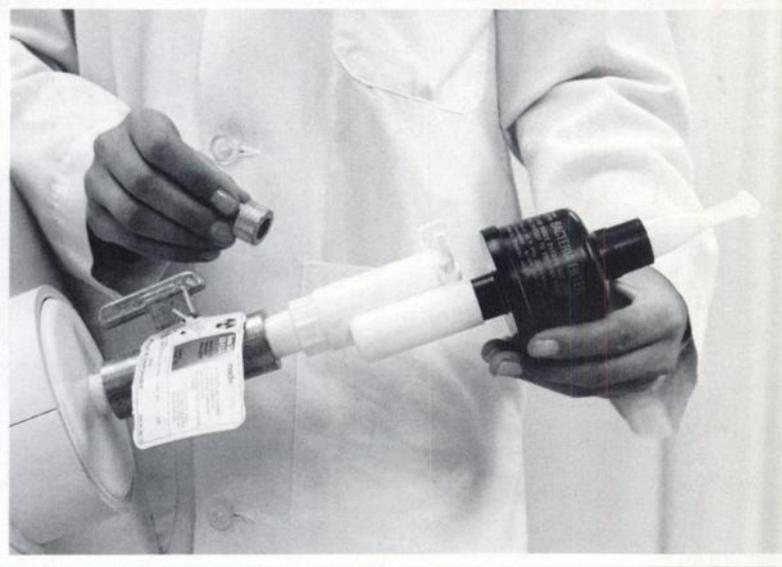

## A versatile, disposable system

Xenon Xe 133-V.S.S. includes everything you need for a Xenon Xe 133 ventilation study. The completely disposable system includes the Xenon Xe 133 contained in a valve-shield, a CO<sub>2</sub> absorber and bag for rebreathing and collection of expired xenon, and a filter/mouthpiece assembly.

One system can be used for single-breath, rebreathing and wash-out studies.

The valve-shield can deliver either a concentrated or a dispersed dose.

## Safe, convenient assembly

Xenon Xe 133-V.S.S. can be assembled in less than a minute. Radiation exposure is minimized because there is no need to dilute the xenon gas or transfer it to a delivery system. After assembly, the ventilation study may begin immediately.

---

**For complete information consult the package insert, a summary of which follows:**

### **Xenon Xe 133-V.S.S. (Xenon Xe 133) Ventilation Study System**



**DESCRIPTION:** The Xenon Xe 133-Ventilation Study System consists of a sealed frangible capsule containing 10 millicuries  $\pm 20\%$  of Xenon Xe 133 gas at calibration time and date with less than 1% carrier xenon in air.

**INDICATIONS AND USAGE:** Study of pulmonary ventilation.

**WARNINGS:** Xenon Xe 133 should not be administered to children or to patients who are pregnant, or to nursing mothers unless the benefits to be gained outweigh the potential hazards. Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

Adequate reproduction studies have not been performed in animals to determine whether this drug affects fertility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Xenon Xe 133 should be used in pregnant women only when clearly needed.

# CONSIDER MPI's XENON Xe 133-V.S.S. (Xenon Xe 133) VENTILATION STUDY SYSTEM

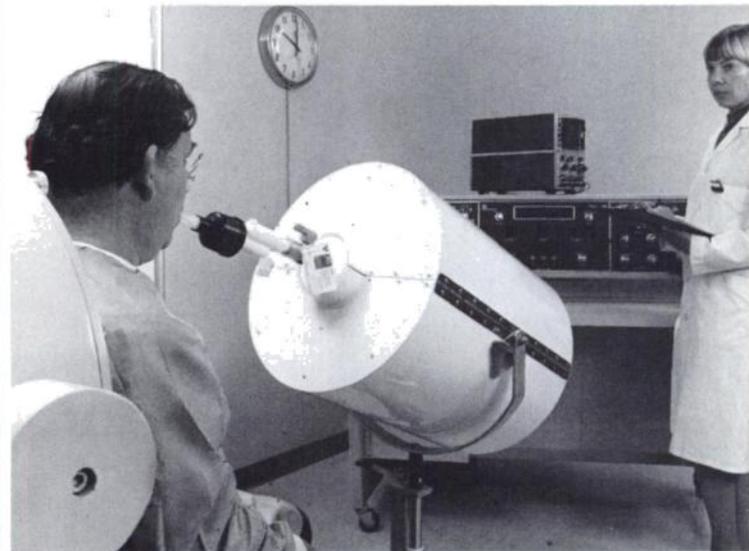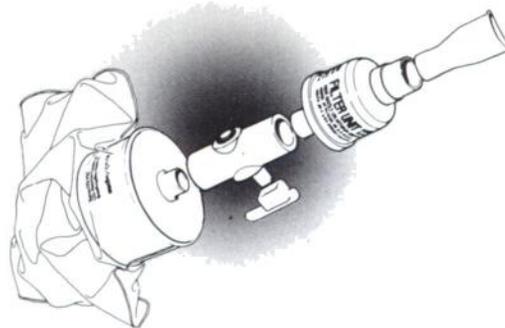

## True, single-unit dose

The MPI Xenon Xe 133-V.S.S. contains enough Xenon Xe 133 for one ventilation study. You only use what you need and are not "locked into" an expensive delivery system that requires daily use to justify costs. Another advantage of single-unit dosage is that the risk of cross infection via reusable apparatus is significantly reduced. Further safety is afforded by the filter/mouth-piece assembly.

## Reduced radiation exposure

The Xenon Xe 133 is supplied in a sealed frangible capsule. The valve-shield is designed to prevent radiation leaks during transport and use. Additionally, a shield to reduce radiation exposure to patient and attending personnel and a valve assembly to minimize the escape of exhaled xenon during washout studies are available as accessory components.

**PRECAUTIONS:** Xenon Xe 133 gas, as well as other radioactive drugs, must be handled with care and appropriate safety measures should be used to minimize radiation exposure to clinical personnel and to patients consistent with proper patient management.

Exhaled Xenon Xe 133 gas should be controlled in a manner that is in compliance with the appropriate regulations of the government agency authorized to license the use of radionuclides.

Xenon Xe 133 gas delivery systems, i.e., respirators or spirometers, and associated tubing assemblies must be leak-proof to avoid loss of radioactivity into the laboratory environs not specifically protected by exhaust systems.

Xenon Xe 133 adheres to some plastics and rubber and should not be allowed to stand in tubing or respirator containers for such unrecognized loss of radioactivity from the dose for administration may render the study non-diagnostic.

**ADVERSE REACTIONS:** Adverse reactions specifically attributable to Xenon Xe 133 have not been reported.

**DOSAGE AND ADMINISTRATION:** The recommended activity range for pulmonary ventilation studies in the average patient (70 kg) is 2 to 20 millicuries (0.03 to 0.3 millicuries/kg).

**HOW SUPPLIED:** Each Ventilation Study System (V.S.S.) contains Xenon Xe 133 in a sealed frangible capsule containing 10 millicuries  $\pm 20\%$  at calibration time and date stated on the label.

The sealed capsule is enclosed in a metal valve-shield which is sealed with a plastic shrink-band to prevent accidental loss of xenon during shipping. A Key is provided to remove the end plugs of the valve-shield and to turn the valve fitting which breaks the sealed capsule of Xenon Xe 133. The V.S.S. also includes a disposable filter/mouthpiece assembly and a breathing-collection bag with an attached CO<sub>2</sub> absorber canister.

Emeryville, California (415) 658-2184.  
Toll Free (In Calif.) (800) 772-2446. (Outside Calif.) (800) 227-0483.

**medi+physics™**

ANOTHER FIRST FROM RADX...



# ISOTRON

## INVENTORY CONTROL COMPUTER

This small desk top microprocessor computer provides complete inventory control and NRC record keeping functions for the nuclear medicine department.

It is user programmable — you program it to fit your requirements even down to the half-life of the radionuclide so the Isotron never becomes obsolete in the rapidly changing field of nuclear medicine.

The Isotron can keep track of up to 20 different radiopharmaceuticals simultaneously by both radionuclide and chemical form! Updates the quantity of radioactivity every minute to reflect radioactivity decay.

The Isotron performs patient dose/volume calculations.

RADX gave you the first calculating dosecalibrator, the first printing dosecalibrator, and now the first desk top inventory control computer, the ISOTRON.



The Isotron subtracts the administered dose from the decayed activity and provides a running total of remaining activity.

The Isotron performs future time calculations. If it is 8:00 A.M. and you want to draw up a dose for 1:00 P.M. the calculation is simply and rapidly performed.

An optional hard copy data printer is available with the Isotron, known as the Isocord, which provides three copies of all pertinent data for your record keeping.

The Isotron may be used with any manufacturer's dosecalibrator.

The Cost? Very reasonable. When combined with the Isocord and our Assayer 1 Dosecalibrator the total price is less than competitive systems with 50% of the capabilities.

For more information or to arrange a demonstration call our toll free number 800-231-1747 (Texas customers call 713-468-9628.)

**RADX**

P. O. Box 19164 Houston, TX 77024

“Make  
the  
best  
available  
better!”



ACTUAL SIZE

“Work on the ultimate, but in the meantime, make the best available better.”

Our people have always accepted the challenge and it's what makes us the leader.

We agree that all things considered the Landauer Gardray 8 film badge system is the best available personnel dosimeter. And, although we are always looking for the ultimate, we have continued to work hard and invest money and time to make it better.


Greatly simplified ordering procedures – permanently encoded unique numbering of film, which is independent of film darkening – new improved techniques for analyzing the film for anomalies that may affect the “meaning” of the exposure and new N.R.C. annual statistical summary reports available now, are just some of the ways our people are working hard to make it better for you.

Write or call for more details.

*Landauer*

R. S. LANDAUER JR. & CO. A  COMPANY  
Glenwood Science Park  
Glenwood, Illinois 60425 . (312) 755-7000

# THE EASY WAY TO YOUR PATIENT'S HEART

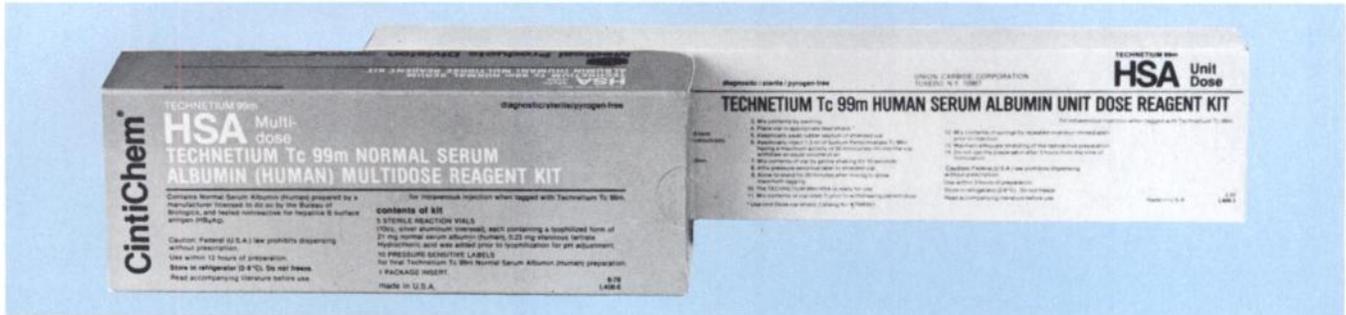

- **RAPID EASY PREPARATION<sup>1</sup>**
- **EXCELLENT BINDING EFFICIENCY<sup>2</sup>**
- **STABLE FORMULATION<sup>2</sup>**
- **CONVENIENT USAGE METHODOLOGY<sup>1</sup>**
- **CONSISTENT RESULTS<sup>2</sup>**
- **UNIT DOSE ECONOMY  
OR MULTIDOSE UTILITY**

For ordering, customer service and technical information call toll-free: (800) 431-1146, until 7:00 p.m. Eastern Standard Time. In New York State, call (914) 351-2131, ext. 227.

**CintiChem<sup>®</sup>**  
TECHNETIUM 99m

## Technetium Tc 99m Normal Serum Albumin (Human) Reagent Kit **HSA** DIAGNOSTIC-FOR INTRAVENOUS USE

### BRIEF SUMMARY OF PRESCRIBING INFORMATION

#### Indications and usage

Technetium Tc 99m Human Serum Albumin is used as an agent for imaging the heart blood pool and to assist in the detection of pericardial effusion and ventricular aneurysm.

#### contraindications

The use of Technetium Tc 99m Human Serum Albumin is contraindicated in persons with a history of hypersensitivity reactions to products containing human serum albumin.

#### warnings

The contents of the kit are not radioactive. However, after the Sodium Pertechnetate Tc 99m is added, adequate shielding of the final preparation must be maintained.

This radiopharmaceutical preparation should not be administered to children or to patients who are pregnant or to nursing mothers unless the expected benefits to be gained outweigh the potential hazards.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of women of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

#### precautions

The components of the kit are sterile and pyrogen-free. It is essential that the user follows the directions carefully and adheres to strict aseptic procedures during preparation of the radiodiagnostic.

Technetium Tc 99m Human Serum Albumin must not be used after three hours from the time of formulation.

Adequate reproduction studies have not been performed in animals to determine whether this drug affects fertility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Technetium Tc 99m Human Serum Albumin should be used in pregnant women only when clearly needed.

It is not known whether this drug is excreted in human milk. As a general rule, nursing should not be undertaken while a patient is on a drug since many drugs are excreted in human milk.

Safety and effectiveness in children have not been established.

Technetium Tc 99m Human Serum Albumin, as well as other radioactive drugs, must be handled with care and appropriate safety measures should be used to minimize external radiation exposure to clinical personnel. Also, care should be taken to minimize radiation exposure to patients, consistent with proper patient management.

The labeling reactions involved in preparing the agent depend on maintaining the tin in the reduced state. Any oxidant present in the Sodium Pertechnetate Tc 99m supply may thus adversely affect the quality of the prepared agent. Hence, Sodium Pertechnetate Tc 99m containing oxidants, or other additives, should not be employed without first demonstrating that it is without adverse effect on the properties of the resulting agent.

#### adverse reactions

Hypersensitivity reactions are possible whenever protein-containing materials such as Technetium Tc 99m labeled human serum albumin are used in man. Epinephrine, antihistamines and corticosteroid agents should be available for use.

#### how supplied

##### unit dose kit

The kit consists of 10 unit dose reaction vials each containing a lyophilized mixture of 7 mg human serum albumin and 0.08 mg stannous tartrate. Hydrochloric acid was added prior to lyophilization for pH adjustment.

##### multidose kit

The kit consists of 5 multidose reaction vials each containing a lyophilized mixture of 21 mg human serum albumin and 0.23 mg stannous tartrate. Hydrochloric acid was added prior to lyophilization for pH adjustment.

### FOR FULL PREPARATION AND PRESCRIBING INFORMATION, SEE PACKAGE INSERTS.

Notes: <sup>1</sup>Refer to package insert for full preparation and prescribing information. <sup>2</sup>Data on file at Union Carbide Corporation, Tuxedo, New York

**UNION CARBIDE** FROM ATOM TO IMAGE

Union Carbide Corporation • Medical Products Division • Nuclear Products • P.O. Box 324 • Tuxedo, New York 10987  
CintiChem is a registered trademark of Union Carbide Corporation.

# The new NEN generator



## We kept it simple and convenient.

Just peel off the top and the new NEN generator is ready for the same top-handling charge-and-elute procedure as current NEN generators.

## We kept it dependable.

Each generator is checked for sterility, apparent Mo 99 breakthrough, alumina breakthrough, and functionality. Pyrogenicity is checked by pooled sample — just like current NEN generators.

## We even kept the same radiation profile... we just made it 10 lbs lighter.

That means about a half ton less total lead you'll have to move around each year — without sacrificing any of the radiation protection delivered by current NEN generators.

For additional information, contact your NEN representative.



**New England Nuclear  
Medical Diagnostics Division**

601 Treble Cove Road  
North Billerica, MA 01862

Call Toll-Free: 800-225-1572

Telex: 94-0996

In Massachusetts and International:  
617-482-9595

# Dependable Performers

## **Minitec<sup>®</sup>** **(Technetium Tc 99m)** **Generator**


Small in size and light in weight, but big in performance. That's Minitec. Designed for minimum amount of exposure to operator, its unique construction (no exposed tubing) and thick shielding (1½" lead) provide high shielding-to-activity ratio. Small-volume, high-concentration eluates give maximum flexibility for varying applications. Wide range of potencies and calibration dates fit the <sup>99m</sup>Tc needs of every lab.

**Minitec (Technetium Tc 99m)**  
**Generator — the largest-selling**  
**generator in the U.S.**

## **Squibb** **Technical** **Associates**



When you buy Minitec and Squibb radiopharmaceuticals, you get the back-up service of a Squibb Technical Associate. He's had extensive training in nuclear medicine, radiopharmaceuticals, RIA and instrumentation. Call him when a new tech needs instruction, a problem develops, you're planning to expand, or there's need for special information. You'll get the prompt, personal attention of an experienced specialist.

**Medotopes<sup>®</sup>**

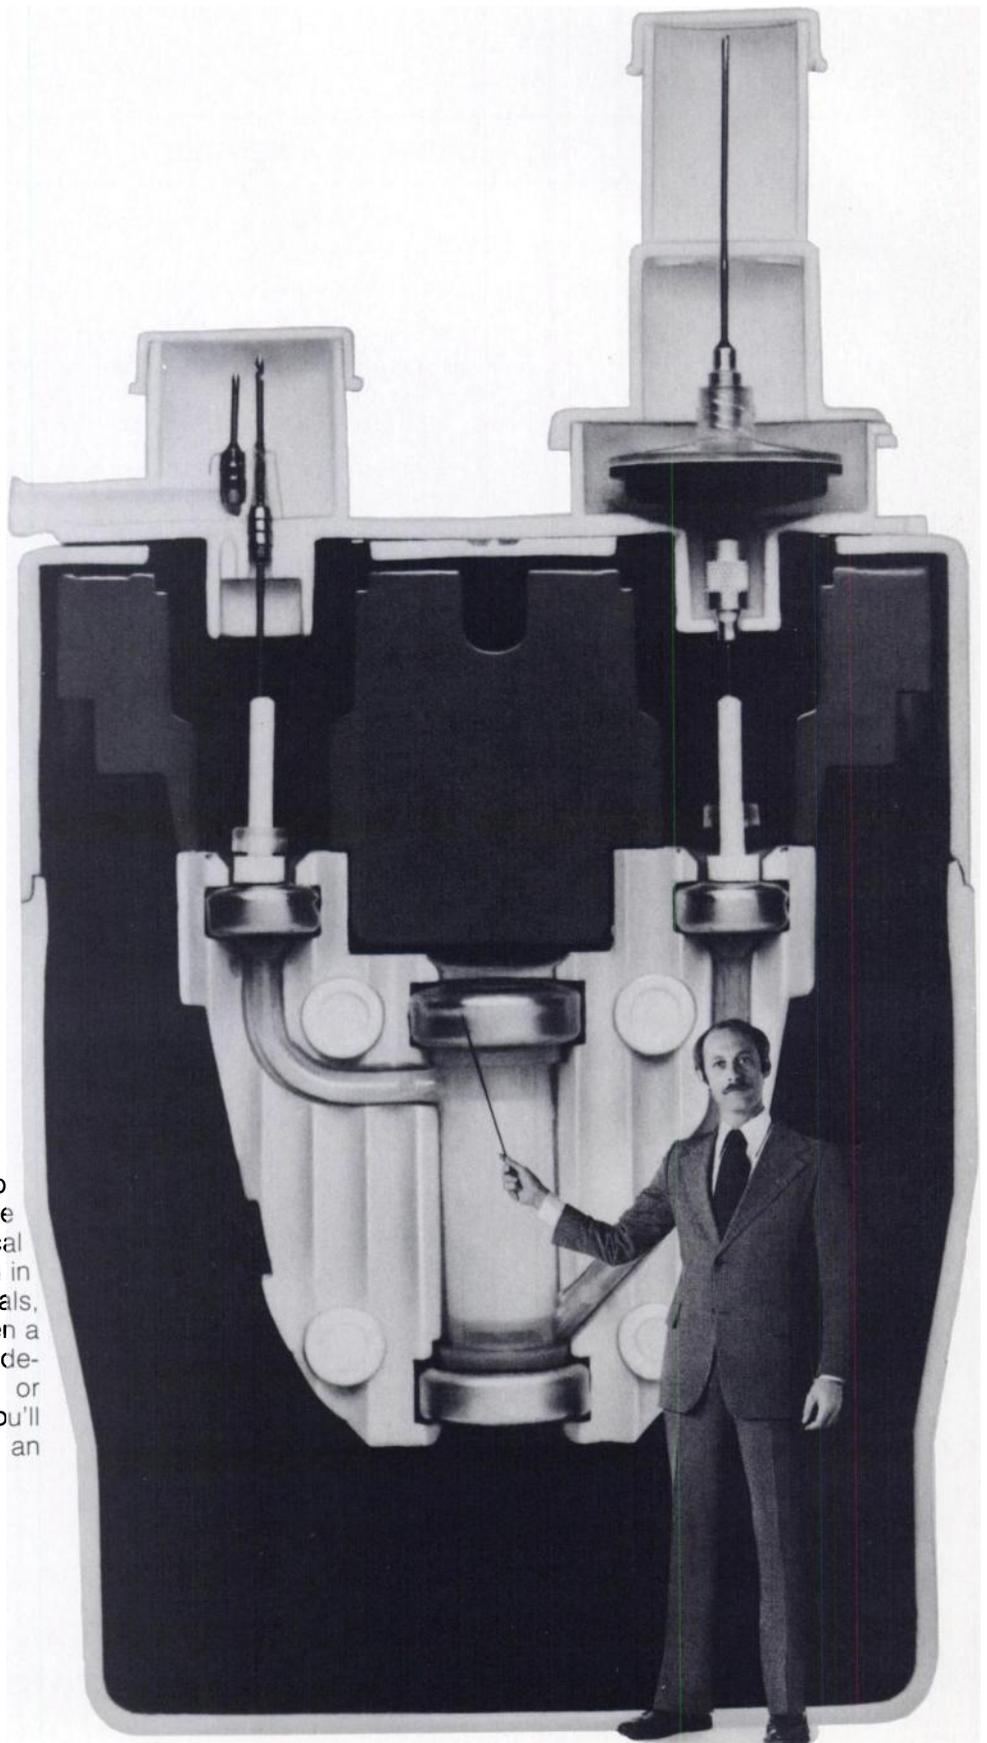


# thrombosis

detection of DVT using I-125 fibrinogen

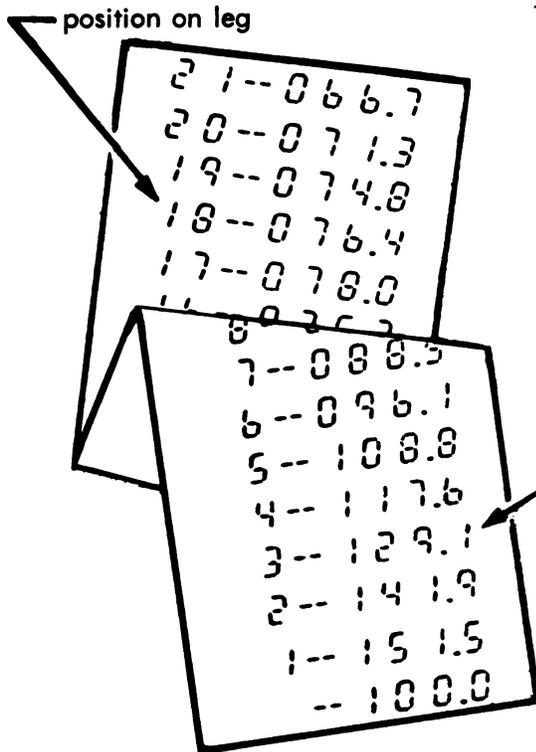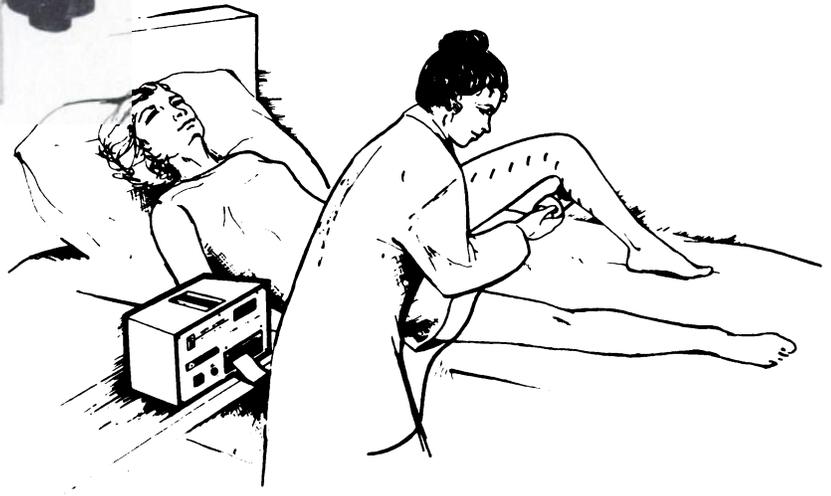

Print Out  
1 1/4 inch wide

- Direct **digital percent** readout
- Printout **saves time**
- **Bedside operation**
- **Right angle probe** minimizes patient disturbance
- Controls are on probe
- Operator **error protection**
- Versatile — settable for other isotopes



**TECHNICAL ASSOCIATES**


7051 ETON AVE. • CANOGA PARK, CA. 91303 (213) 883-7043

# Gamma Camera Upgrade

**1/10 Inch or Better Resolution at a fraction of new system cost.**

**BEFORE**

NEN Thallium 201 phantom at 2" distance from collimator.  
500K

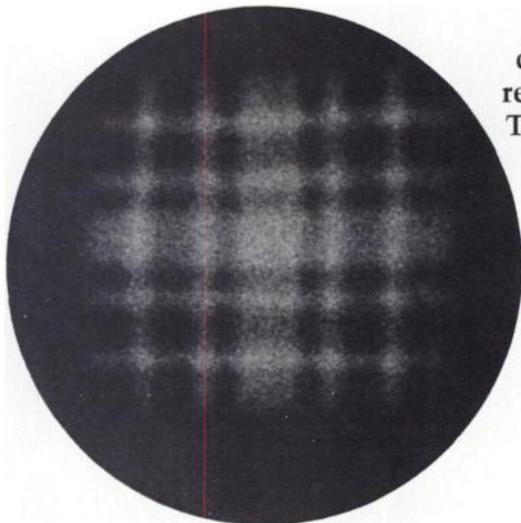

Picker 2C with ultrafine collimator.

Enjoy new camera performance without a major investment. Nuclear Service Inc. can upgrade your existing gamma camera system to provide you with 1/10" or better intrinsic resolution.

With NSI upgrade you not only receive State-of-the-Art resolution, but in most cases you


**The picture on your left does not provide adequate resolution for cardiac work. The picture on the right is more than adequate!**

converted system will provide you with **IMPROVED FIELD UNIFORMITY.**

Learn more about this efficient and economical method available from one of the country's largest independent nuclear medicine service organizations. Call or write NSI for complete infor-

**AFTER**

NEN Thallium 201 phantom at 2" distance from collimator.  
500K

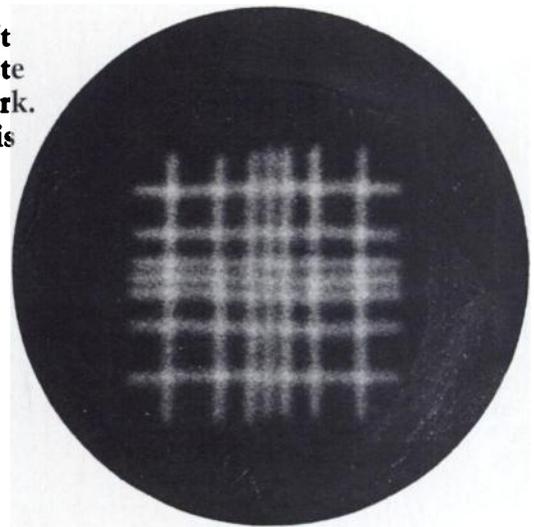

Picker 2C with ultrafine collimator and SX-11 detector head.

mation on gamma camera upgrade.

Up to 75% Better Resolution.

Picker	Improved Resolution
2	75%
2C	50%
3C, 4-12	40%
1/8"	20%


\*Leasing plans and reconditioned upgraded systems also available.

**Nuclear Services Inc.**



Nuclear Services Inc. (516) 752-9270  
P. O. Box 5492 (203) 281-3957  
Hamden, CT 06518

# REDUCE YOUR WITH THE ECONOMIC ALTERNATIVES

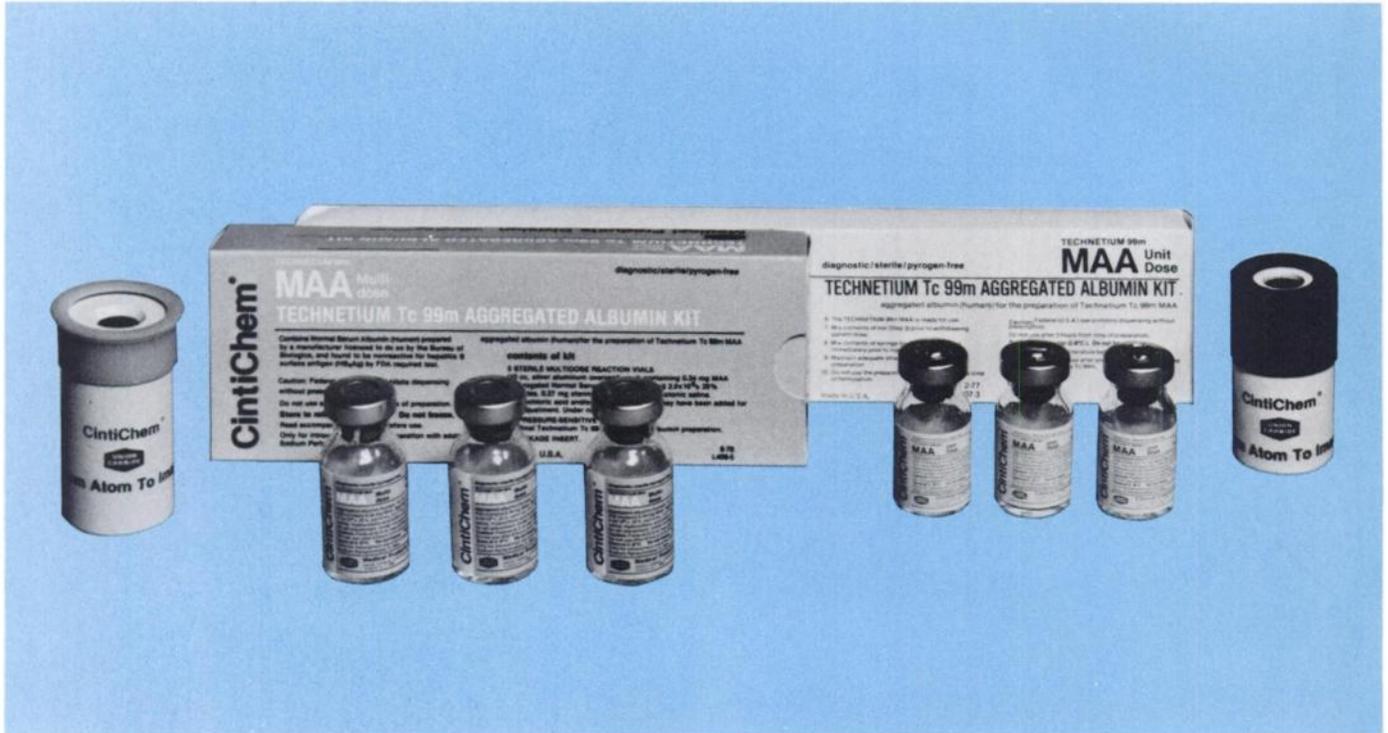

**THE ECONOMIC ALTERNATIVES**, available only from UNION CARBIDE NUCLEAR PRODUCTS, consist of diagnostic kits such as **CINTICHEM® TECHNETIUM 99m MAA** in **UNIT DOSE** and **MULTIDOSE** vial sizes, designed for the full range of dose preparation needs required to meet today's practice of Nuclear Medicine in an environment of cost containment.

**CINTICHEM® TECHNETIUM 99m MAA UNIT DOSE** and **MULTIDOSE** both offer the following advantages:

- **EASY TO PREPARE<sup>1</sup>**
- **STABLE FORMULATION**—Prepared with Stannous Tartrate<sup>2</sup>, which is more resistant to oxidation than Stannous Chloride.
- **LOWEST DOSE RATE TO THE LUNGS OF ANY COMMERCIALY AVAILABLE KIT<sup>3</sup>**

# IMAGING COSTS

## AVAILABLE ONLY FROM UNION CARBIDE

**CINTICHEM® TECHNETIUM 99m MAA UNIT DOSE** can reduce the cost of operating any size patient volume department:

**UNIT DOSE** kits each contain 10 vials

**UNIT DOSE** kits are competitively priced with 5 vial multidose kits

**UNIT DOSE** can reduce the cost of operating any department when maintained in inventory and substituted for a multidose vial on a single unexpected special, late afternoon, or weekend study, when a prepared multidose vial is not available

**UNIT DOSE** kits can reduce your average cost per dose if an average of one perfusion study is routinely performed per day; ideal for low volume departments

**CINTICHEM® TECHNETIUM 99m MAA MULTIDOSE**, for use with up to 90 mCi per vial, can provide moderate to high patient volume departments with the optimum economical dosage availability from a single vial.

<sup>1</sup> See Union Carbide CintiChem® Technetium 99m MAA Unit Dose or Multidose package insert for full preparation instructions.

<sup>2</sup> Union Carbide Reg. U.S. Patent Office # 3987157

<sup>3</sup> Refer to Union Carbide and competitive package inserts for full lung dosimetry information.

TO ORDER OR FOR ADDITIONAL INFORMATION

CALL  
TOLL  
FREE

# 800-431-1146

IN N.Y.S. CALL (914) 351-2131 EXT 227

You can also take advantage of the other **CINTICHEM® ECONOMIC ALTERNATIVES** by ordering today Unit Dose and/or Multidose **Technetium 99m DTPA** (DTPA Tin Kit For Use In The Preparation of Technetium Tc 99m DTPA Tin Chelate) and **Technetium 99m HSA** (Technetium Tc 99m Serum Albumin (Human) Reagent Kit).

**THE ECONOMIC ALTERNATIVES** such as **CINTICHEM® TECHNETIUM 99m MAA UNIT DOSE** and **MULTIDOSE** (Technetium Tc 99m Aggregated Albumin Kit), can be utilized to maximum economic advantage by preparation of the vial size that best meets your daily scheduling and immediate dosage needs.

With a **CINTICHEM® STANDING ORDER** (the original "convenience packaging") you can mix your purchase and delivery of CintiChem® 10 vial **UNIT DOSE** and 5 vial **MULTI DOSE** kits at the same competitive price.

Compared to competitive "convenience packaging", a CintiChem® Standing Order allows you to optimize your kit purchases and delivery schedule to meet your individual dosage needs; reduces your shelf space requirements; and continuously assures you of product with the longest expiration date available.

**CINTICHEM®**  
TECHNETIUM 99M

**MAA** Technetium Tc 99m  
Aggregated Albumin Kit



**FROM ATOM TO IMAGE**

Union Carbide Corporation • Medical Products Division • Nuclear Products • P.O. Box 324 • Tuxedo, New York 10987

CintiChem is a registered trademark of Union Carbide Corporation



# CintiChem

TECHNETIUM 99m

# MAA Technetium Tc 99m Aggregated Albumin Kit

## BY ALL INDICATIONS; THE SOLUTION FOR YOUR LUNG IMAGING NEEDS

### BRIEF SUMMARY OF PRESCRIBING INFORMATION

#### Indications and usage

Technetium Tc 99m Aggregated Albumin is indicated as a lung imaging agent to be used as an adjunct in the evaluation of pulmonary perfusion.

#### contraindications

Technetium Tc 99m Aggregated Albumin should not be administered to patients with severe pulmonary hypertension.

The use of Technetium Tc 99m Aggregated Albumin is contraindicated in persons with a history of hypersensitivity reactions to products containing human serum albumin.

#### warnings

The possibility of allergic reactions should be considered in patients who receive multiple doses.

Theoretically, the intravenous administration of any particulate material such as aggregated albumin imposes a temporary small mechanical impediment to blood flow. While this effect is probably physiologically insignificant in most patients, the administration of aggregated albumin is possibly hazardous in acute *cor pulmonale* and other states of severely impaired pulmonary blood flow.

This radiopharmaceutical preparation should not be administered to children, to pregnant women or lactating women unless the expected benefits to be gained outweigh the potential risks.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

#### precautions

In cases of right-to-left cardiac shunt, additional risk may exist due to the rapid entry of aggregated albumin into the systemic circulation.

The contents of the kit are not radioactive. However, after the Sodium Pertechnetate Tc 99m is added, adequate shielding of the final preparation must be maintained.

The labeling reactions involved in preparing the agent depend on maintaining the tin in the reduced state. Any oxidant present in the Sodium Pertechnetate Tc 99m supply may thus adversely affect the quality of the prepared agent. Hence, Sodium Pertechnetate Tc 99m containing oxidants, or other additives, should not be employed without first demonstrating that it is without adverse effect on the properties of the resulting agent.

The contents of the vial are sterile and pyrogen-free. It is essential that the user follows the directions carefully and adheres to strict aseptic procedures during preparation of the radiodiagnostic.

Technetium Tc 99m Aggregated Albumin is physically unstable and as such the particles will settle with time. Failure to agitate the vial adequately before use may result in non-uniform distribution of radioactivity.

It is also recommended that, because of the increasing probability of agglomeration with aging, a batch of Technetium Tc 99m Aggregated Albumin not be used after eight hours from the time of preparation. Refrigerate at 2° to 8° C after preparation. If blood is withdrawn into the syringe, unnecessary delay prior to injection may result in clot formation *in situ*.

The contents of the vial are under a nitrogen atmosphere and should be protected from air. On preparation with Sodium Pertechnetate Tc 99m, the contents of the vial should be mixed by gentle swirling to avoid changes in particle size. Do not use if clumping or foaming of the contents is observed.

Adequate reproduction studies have not been performed in animals to determine whether this drug affects fertility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Technetium Tc 99m Aggregated Albumin should be used in pregnant women only when clearly needed.

It is not known whether this drug is excreted in human milk. As a general rule, nursing should not be undertaken while a patient is on a drug since many drugs are excreted in human milk.

Safety and effectiveness in children have not been established.

As in the use of any radioactive material, care should be taken to minimize radiation exposure to the patient, consistent with proper patient management, and to insure minimum radiation exposure to the occupational worker.

Radiopharmaceuticals should be used only by physicians who are qualified by training and experience in the safe use and handling of radionuclides and whose experience and training have been approved by the appropriate governmental agency authorized to license the use of radionuclides.

#### adverse reactions

The literature contains reports of deaths occurring after the administration of aggregated albumin to patients with pre-existing severe pulmonary hypertension. Instances of hemodynamic or idiosyncratic reactions to preparations of Technetium Tc 99m labeled aggregated albumin have been reported.

Hypersensitivity reactions are possible whenever protein-containing materials such as Technetium Tc 99m labeled aggregated albumin are used in man. Epinephrine, antihistamines and corticosteroid agents should be available for use.

#### how supplied

##### unit dose kit

The kit consists of 10 unit dose reaction vials, each containing 0.11 mg of Aggregated Normal Human Serum Albumin (MAA), 0.09 mg stannous tartrate, and 0.3 ml of isotonic saline. Hydrochloric acid and/or sodium hydroxide may have been added for pH adjustment. Each vial contains 0.5 - 1.0 X 10<sup>6</sup> aggregated albumin particles.

##### multidose kit

The kit consists of 5 multidose reaction vials, each containing 0.34 mg of Aggregated Normal Serum Albumin (Human) MAA, 0.27 mg stannous tartrate, and 0.6 ml of isotonic saline. Hydrochloric acid and/or sodium hydroxide may have been added for pH adjustment. Each vial contains 2.0 X 10<sup>6</sup> ±25% aggregated albumin particles.

FOR FULL PREPARATION AND PRESCRIBING INFORMATION, SEE PACKAGE INSERT

# **Save up to 40% on your next Camera System**

*Utilize NOVA Medical Systems' unique approach to generic purchasing.*


*NOVA Medical Systems buys Collimators direct. They are identical to those supplied by gamma scintillation camera manufacturers.*

*NOVA's collimators not only meet the same specifications, but are warranted for five years. NOVA Medical offers a money-back guarantee with every purchase!*

*Why pay a markup to camera manufacturers for Collimators they don't produce?*

*Save on your next purchase. Inquire about the wide range of products and services available through NOVA's generic purchasing program.*


*Call Collect. 312-843-7600*

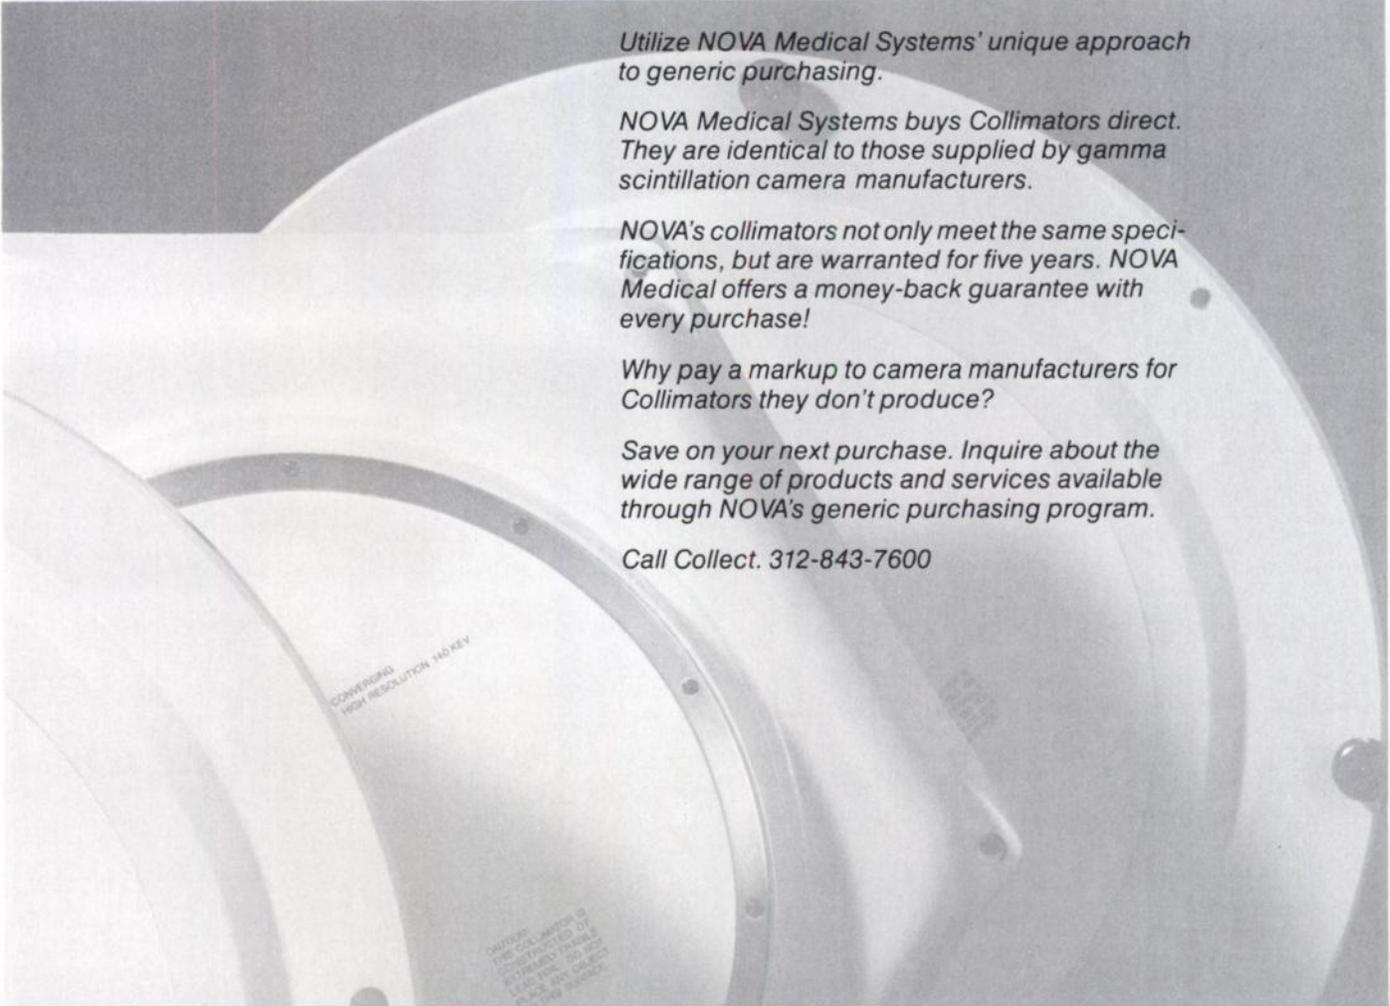

**NOVA MEDICAL**

**NOVA Medical Systems, Ltd.**  
1701 E. Woodfield Drive  
Schaumburg, IL 60195

# Do something else with your lab's boiling water.

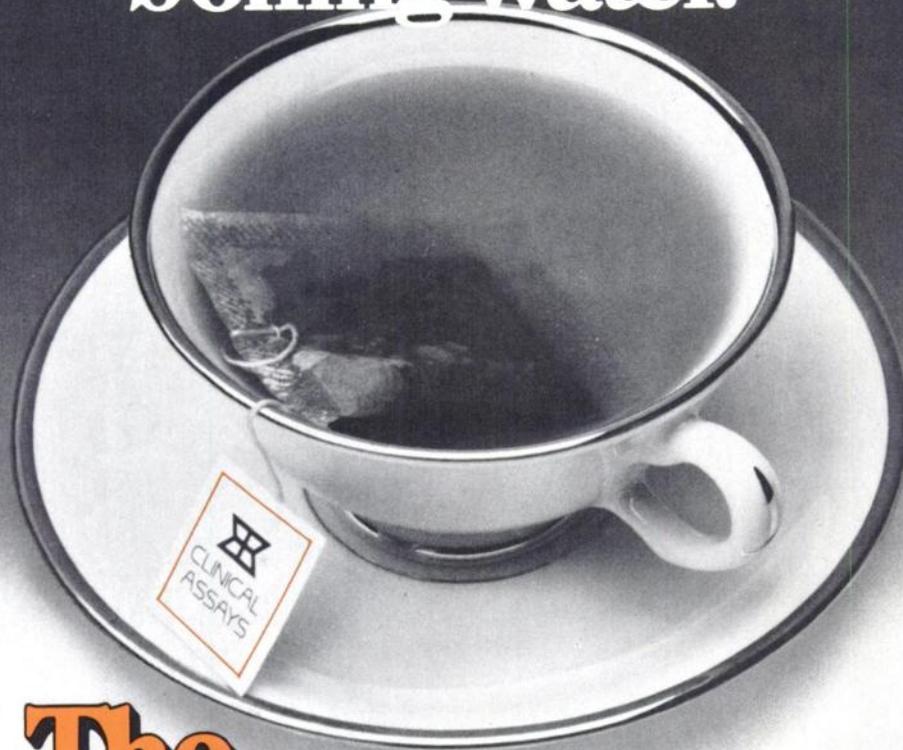

## The No-Boil Folate

## New GammaDab<sup>®</sup> [<sup>125</sup>I] Folate Radioassay Kit

- Room temperature denaturation eliminates boiling
- New technology combines binder and separator into one reagent
- No charcoal
- Single tube assay—less than 30 minutes technician time
- Human serum N<sup>5</sup>-MTHFA standards
- Typically greater than 94% recovery of N<sup>5</sup>-MTHFA at all levels

Send for more information today.


 **CLINICAL ASSAYS**  
DIVISION OF TRAVENOL LABORATORIES, INC.

620 Memorial Drive, Cambridge, MA 02139  
(617) 492-2526 • TWX: 710-320-6460  
Toll free outside Mass: (800) 225-1241

For other worldwide locations, please contact your local Clinical Assays/Travenol representative or the International Sales Department, Clinical Assays, Cambridge, MA 02139 U.S.A.

Complete directions are provided with each product. These directions should be read and understood before use. Particular attention should be paid to all warnings and precautions. Additional performance data are available. Should you have any questions, contact your Clinical Assays/Travenol representative.

Patent pending.

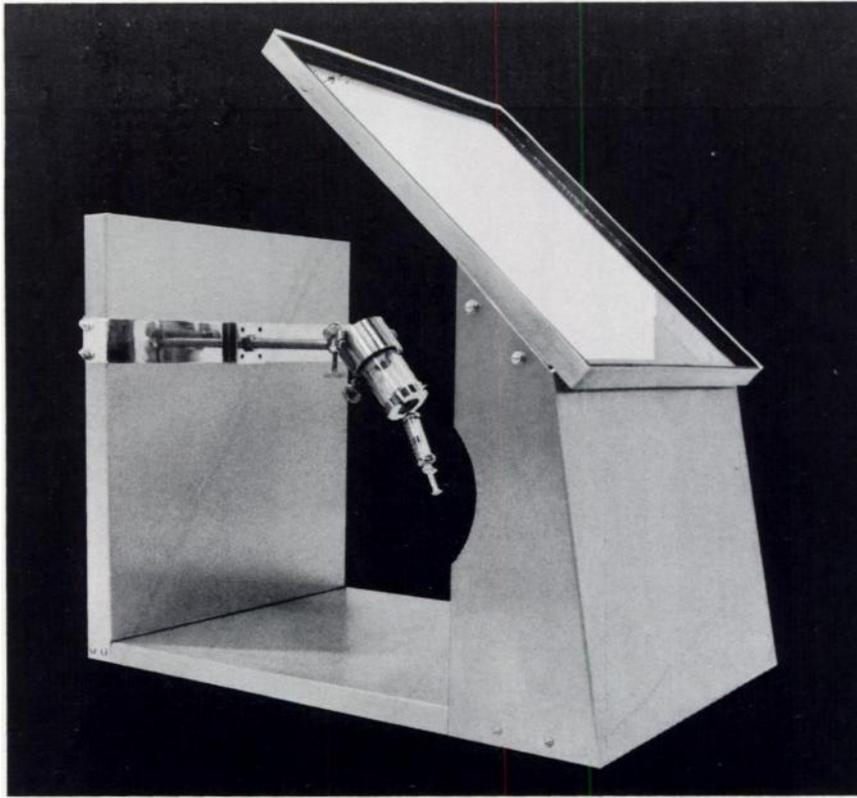

## Now there's a Radiation Dose Shield that offers more than just protection.

Safety, versatility and convenience. Nuclear Pacific's new Radiation Dose Shield provides all three through an expandable, modular design that allows you to select exactly the features your working environment most requires.

The basic stand consists of a 16"x 18" cantilevered frame holding 1/4" (4.8 density) lead glass, vertical stainless steel-clad forward wall and a horizontal work surface. The forward wall contains 3/8" lead lining. The basic unit can be ordered with thicker and higher density glass (the frame accommodates thicknesses up to 1") and/or with a vial-shield-holding back wall. (As shown.)

Basic unit size is 17" wide by 25" deep and is 25" high. Net weight: 129 lbs.

**Radiation Dose Shield Model 30**  
**Basic Unit** \$498.00  
 includes:

Front Stainless Steel with 3/8" Lead  
 Side Stainless Steel with 3/8" Lead  
 Bottom Stainless Steel only  
 Frame with 4.8 density 1/4" Lead Glass


Select the basic unit or any of these options:

Options: Add prices below to base unit, Model 30 price

Model 31 - A	Back-Stainless Steel Panel	\$ 68.00
Model 31 - B	Back-3/8" Lead Sheet	\$ 64.00
Model 31 - C	Bottom 3/8" Lead Sheet	\$ 86.00
*Model 31 - D	Utility Bar	\$ 90.00
Model 31 - 75	Lo Energy Vial Shield Holder	\$ 50.00
Model 31 - 77	Hi Energy Vial Shield Holder	\$ 50.00
Model 31 - 79	Ultra Hi Energy Vial Shield Holder	\$ 50.00
Model 31 - 481	1/2" 4.8 Density Lead Glass	\$ 63.00
Model 31 - 622	1/2" 6.2 Density Lead Glass	\$100.00
Model 31 - 623	3/4" 6.2 Density Lead Glass	\$175.00
Model 31 - 624	1" 6.2 Density Lead Glass	\$275.00

\*Only one required for 1 to 4 Vial Shield Holders.


To order, contact Nuclear Pacific, Inc., (206) 763-2170.

**Nuclear  
 Pacific,  
 Inc.** 


6701 Sixth Ave. S. Seattle, WA 98108

# A complete nuclear image

As the uses for nuclear medicine continue to expand, the responsibilities of the nuclear physician and the radiologist will increase just as rapidly. Their services are requested in more and more disciplines. Picker gamma-camera systems have been designed to allow the physician to select and refine the views he needs. Picker Dyna®Camera accessories help our cameras to see more. As our systems have grown more sophisticated in their ability to deliver results, they've also become simpler to use and maintain.

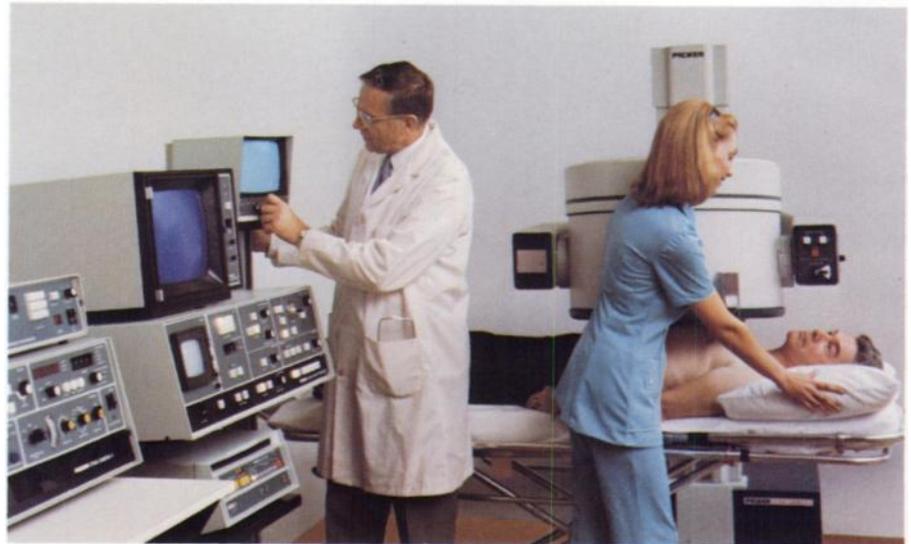

**DynaCamera 4/15 takes the large view.** Within the DynaCamera 4 series, Picker's 4/15 becomes the nucleus of a nuclear medicine department. Its 15" (380 mm) detector brings high uniformity and exceptional system resolution.

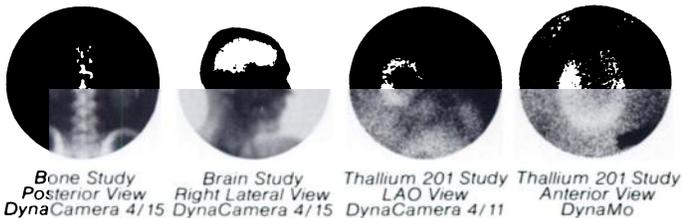


Bone Study  
Posterior View  
DynaCamera 4/15

Brain Study  
Right Lateral View  
DynaCamera 4/15

Thallium 201 Study  
LAO View  
DynaCamera 4/11

Thallium 201 Study  
Anterior View  
DynaMo

It can image lung and liver/spleen studies in one view — without a diverging collimator. It's ideal for cerebral and cardiac flow studies, lung perfusion studies, bone, liver/pancreas and kidney studies.

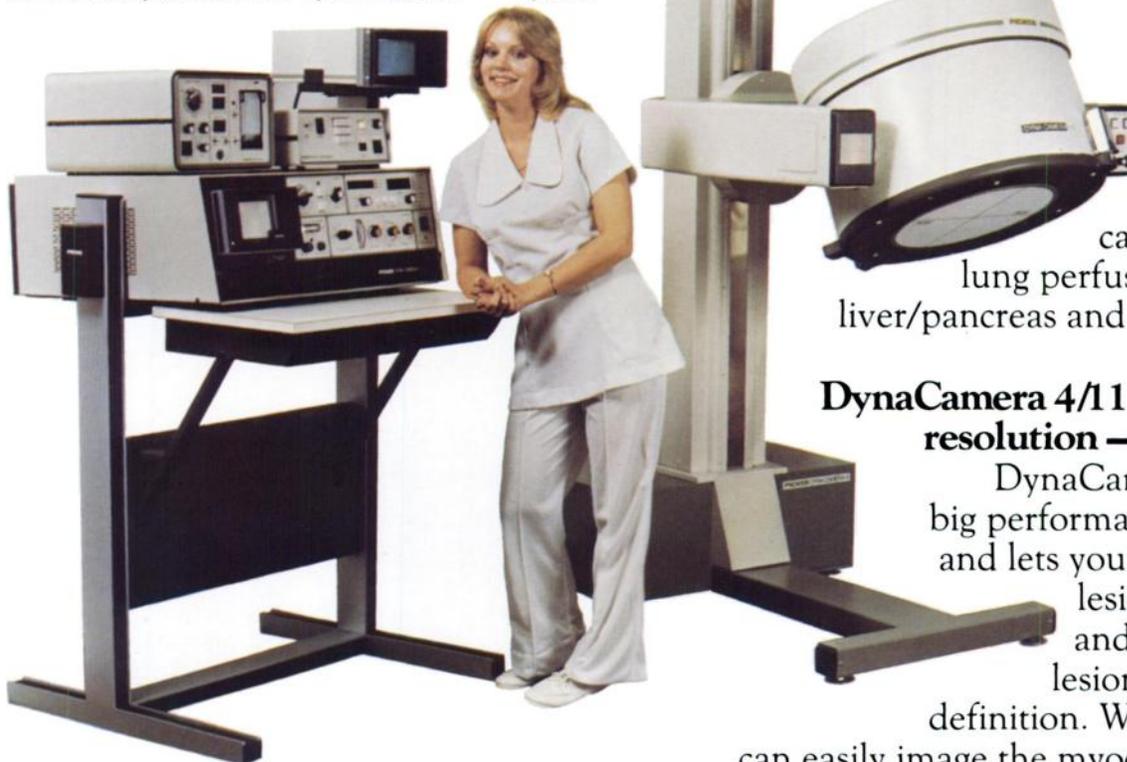


**DynaCamera 4/11 for unparalleled resolution — 3.6 mm FWHM.**

DynaCamera 4/11 delivers big performance in small areas, and lets you visualize small lesions, often hidden, and shows larger lesions with clearer definition. With the 4/11, you

can easily image the myocardium to locate and measure infarcts, get precise region placement in left ventricular ejection fraction studies, and obtain cardiac-output measurements.

# needs a complete system.

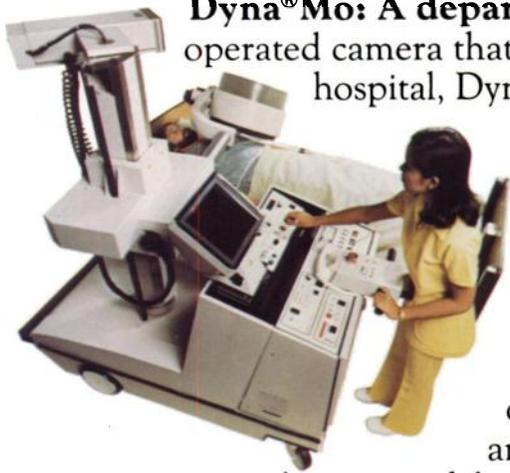


**Dyna<sup>®</sup>Mo: A department on wheels.** As a high-resolution, mobile, battery-operated camera that extends the role of nuclear medicine to every part of the hospital, DynaMo is a great system to have around. Its high-resolution detector — 3.6 mm FWHM — makes it the equal of our finest small field of view cameras and its quick-change collimators, five-motion detector and integral tape recorder make it a virtual department in itself.


**DynaCamera accessories expand the role of your department in important new directions.** Your selection of the right DynaCamera 4 gives you the range of capabilities your nuclear medicine department needs — and your selection of the right DynaCamera 4 accessories takes even greater advantage of these capabilities. For example, our Cardiac Module used in conjunction with DynaMo or any DynaCamera 4 system, allows you to compute



left-ventricular ejection fraction without the expensive services of a nuclear computer. Our Clinical Image Processor significantly improves upon your present methods of viewing, analyzing, photographing and recording

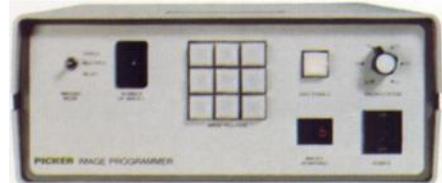

images. The Picker Image Programmer makes it possible to record multiple images on a single piece of film. Our Compact Recording Camera, used with PIP, formats and photographs up to 90 images on a single film. And, we offer the widest selection of collimators in the industry, to give you the best speed, resolution, sensitivity and convenience.

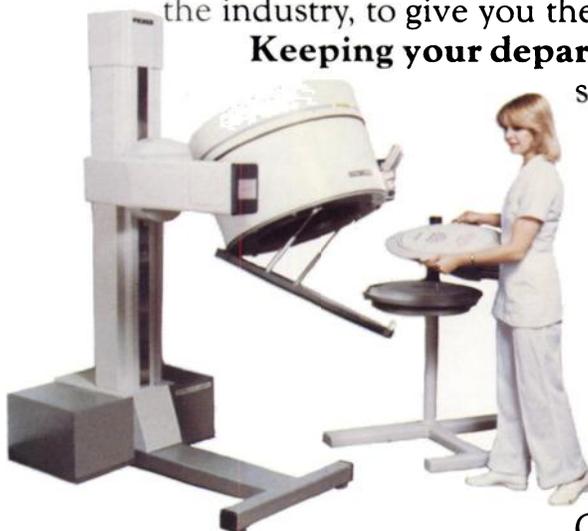

**Keeping your department ahead of the future.** A modular DynaCamera 4 system is an investment in the future of nuclear medicine. As new technologies emerge from the laboratory, Picker gamma-camera systems will keep pace . . . and set it. Our investment in the future of nuclear medicine is rooted in 20 years of industry leadership through the concept of adding capabilities, not complications.

For full details, contact Picker Corporation,  
12 Clintonville Road, Northford, CT 06472  
(203-484-2711); or  
Picker International,  
595 Miner Road,  
Cleveland, OH 44143.

**PICKER<sup>®</sup>**

ONE OF THE C.I.T. COMPANIES



**For its size, the NE 1600  
has a great track record**



Very high through-put, simplicity of operation, exceptional reproducibility, excellent performance, reliability and compactness are major factors in the world wide success so quickly achieved by NE 1600  $^{125}\text{I}/^{57}\text{Co}$  Counter. In laboratories engaged in routine testing and in research, the outstanding ability of the NE 1600 to count large numbers of samples in a short period of time is widely recognised. A count of 240 typical samples, for 30 seconds each, takes only 8 minutes to complete with the NE 1600, compared with 3 hours 30 minutes in an automatic gamma counter.

**NE NUCLEAR ENTERPRISES LIMITED**



Sighthill Edinburgh, EH11 4EY  
Scotland. Tel: 031-443 4060 Telex 72333  
Cables—Nuclear Edinburgh.

Associate Companies:

N. E. Nuclear Enterprises,  
25 Chemin François—Lehmann  
1218 Grand Saconnex, Genève.  
Tel (022) 98-16-61/62 Telex 289066

Nuclear Enterprises GmbH  
Schwanthalerstrasse 74.  
8 München 2, Germany  
Tel: 53-62-23 Telex 529938

## DIAGNOSTIC ISOTOPES MDP KIT TECHNETIUM Tc 99m MEDRONATE KIT

### INDICATIONS AND USAGE

Technetium Tc 99m Medronate may be used as a bone imaging agent to delineate areas of altered osteogenesis.

### CONTRAINDICATIONS

None known.

### WARNINGS

This class of compound is known to complex cations such as calcium. Particular caution should be used with patients who have, or who may be predisposed to, hypocalcemia (i.e., alkalosis).

This radiopharmaceutical drug product should not be administered to children, to pregnant women, or to nursing mothers, unless the expected benefit to be gained outweighs the potential risk.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

### PRECAUTIONS

#### General

Technetium Tc 99m Medronate as well as other radioactive drugs, must be handled with care and appropriate safety measures should be used to minimize radiation exposure to clinical personnel. Also, care should be taken to minimize radiation exposure to the patients consistent with proper patient management.

To minimize radiation dose to the bladder, the patient should be encouraged to void when the examination is completed and as often thereafter as possible for the next 4-6 hours.

This preparation contains no bacteriostatic preservative.

Technetium Tc 99m Medronate should be formulated within six (6) hours prior to clinical use.

#### Pregnancy Category C

Adequate reproductive studies have not been performed in animals to determine whether this drug affects fertility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Technetium Tc 99m Medronate should be used in pregnant women only when clearly needed.

#### Nursing Mothers

It is not known whether this drug is excreted in human milk. As a general rule nursing should not be undertaken while a patient is on the drug since many drugs are excreted in human milk.

#### Pediatric Use

Safety and effectiveness in children have not been established.

### ADVERSE REACTIONS

No adverse reactions specifically attributable to the use of Technetium Tc 99m Medronate have been reported.

### DOSAGE AND ADMINISTRATION

The suggested dose range for i.v. administration, after reconstitution with oxidant-free sodium pertechnetate Tc 99m Injection, to be employed in the average patient (70 kg) is:

Bone imaging: 10-20 mCi Technetium Tc 99m Medronate

Scanning post-injection is optimal at about 1-4 hours.

Slow administration of the drug over a period of 30 seconds is recommended.

The patient dose should be measured by a suitable radioactivity calibration system immediately prior to administration.

Radiopharmaceuticals should be used only by physicians who are qualified by training and experience in the safe use and handling of radionuclides and whose experience and training have been approved by the appropriate government agency authorized to license the use of radionuclides.

### HOW SUPPLIED

Diagnostic Isotopes' Technetium Tc 99m Medronate Kit is supplied as a sterile, pyrogen-free kit containing 10 vials.


Each 10 ml vial contains 10 mg medronic acid, 0.17 mg (minimum) stannous chloride (maximum stannous stannic chloride 0.29 mg), and 2 mg ascorbic acid. The pH has been adjusted to 4-8 with either HCl or NaOH prior to lyophilization. Following lyophilization, the vials are sealed under a nitrogen atmosphere.

For Superior Bone Images\*

# DIAGNOSTIC ISOTOPES MDP

(Technetium Tc 99m Medronate Kit)

**Our Formulation Is Not The Same!  
Only Diagnostic Isotopes MDP  
Contains Ascorbic Acid**

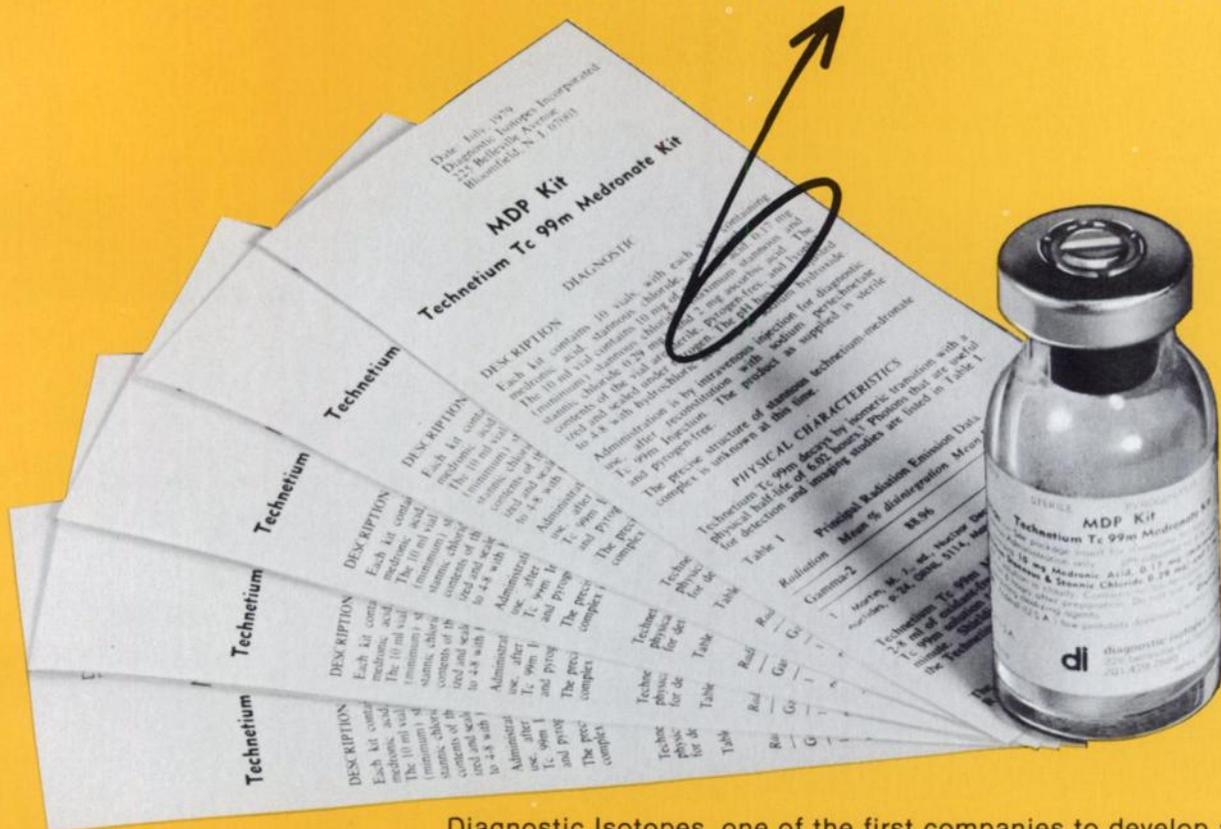

Diagnostic Isotopes, one of the first companies to develop a Technetium labeled bone imaging agent, is proud to announce its new MDP Kit. Physicians who are acquainted with D.I. quality and service will welcome this latest addition to our product line. As with all D.I. reagents, MDP is conveniently packaged in 10 multi-dose vial kits which may be stored at room temperature.

For pricing information and prompt service, please call either of the numbers listed below.

\*G. Subramanian, et al: Technetium-99m Methylene Diphosphonate — A superior agent for skeletal imaging. Comparison with other Technetium complexes. J. Nucl Med 16:74, 1975

**di**

**diagnostic isotopes incorporated**

225 Belleville Avenue, Bloomfield, NJ 07003

Toll free (800)631-1260, (201)429-7590, Telex 133393 Diagnostic BLFD

See Opposite Page For Summary Of Prescribing Information

**TWO NEW KITS FROM  
INTERNATIONAL CIS  
THE WIDE RANGE OF QUALITY RIA PRODUCTS  
FROM INTERNATIONAL CIS IS NOW FURTHER  
EXTENDED BY NEW KITS FOR**

**FERRITIN**  
**TRYPSIN**

**FERRITIN**

for determination of total iron status

**TRYPSIN**

for investigation of pancreatic function and diagnosis of pancreatitis



for further details contact :

**INTERNATIONAL CIS** / 2, rue Stephenson / 78181 St Quentin - Yvelines Cedex France / Tél. (33) (1) 043.00.09 / Telex 698226 F

**CIS RADIOPHARMACEUTICALS Inc.** / 5, de Angelo Drive / Bedford-Mass 01730 - USA / Tél. (617) 275.7120 / Telex 0949465

**EUROTOPE SERVICES Ltd.** / Rex House - 354 Ballards Lane / North Finchley - London - N 12 OEG GB / Tel. (01) 446.4405 / Telex 23310

**ISOTOPEN DIENST WEST** / Einsteinstrasse 9-11 / 6072 - Dreieich bei Frankfurt-Main Germany / Tel. (06103) 3857 / Telex 4185312

Not presently available in USA, awaiting FDA approval.

# Xenon Found in Room Air By 80% of <sup>133</sup>Xe Users

80% of a sample of XenAlert™ owners reported finding xenon gas releases of which they were previously unaware. Discovery of varying xenon concentrations during "routine" ventilation studies had been virtually impossible to detect prior to using the "XenAlert" Xenon-133 Monitor.



## XenAlert™

## Xenon-133 Room Air & Trap Monitor\*

The **ONLY** instrument that integrates the xenon-133 concentration (MPC · HRS) for a full week, as required by NRC and Agreement States.<sup>1</sup>

- Audible and visual indicators alert you BEFORE a hazardous xenon concentration is reached.
- Ideal for workers in restricted areas.
- Monitors and displays <sup>133</sup>Xe concentration exiting from gas trap to indicate when filter cartridge needs replacement.
- Recorder output for keeping permanent records.

**SATISFACTION GUARANTEED OR MONEY REFUNDED.**  
*Demonstrations available.*

Send for full details.  
Ask for Bulletin 266-B



### NUCLEAR ASSOCIATES


Division of VICTOREEN, INC.

100 Voice Road • Carle Place, N.Y. 11514 • (516) 741-6360

<sup>(1)</sup>The Code of Federal Regulations† clearly limits the permissible <sup>133</sup>Xe exposure to 1 MPC for 40 hours per week for 13 weeks. The data is continuously updated and displayed by the "XenAlert."

† 10 CFR, Part 20, Sec. 20.103 and Appendix B, Table 1.



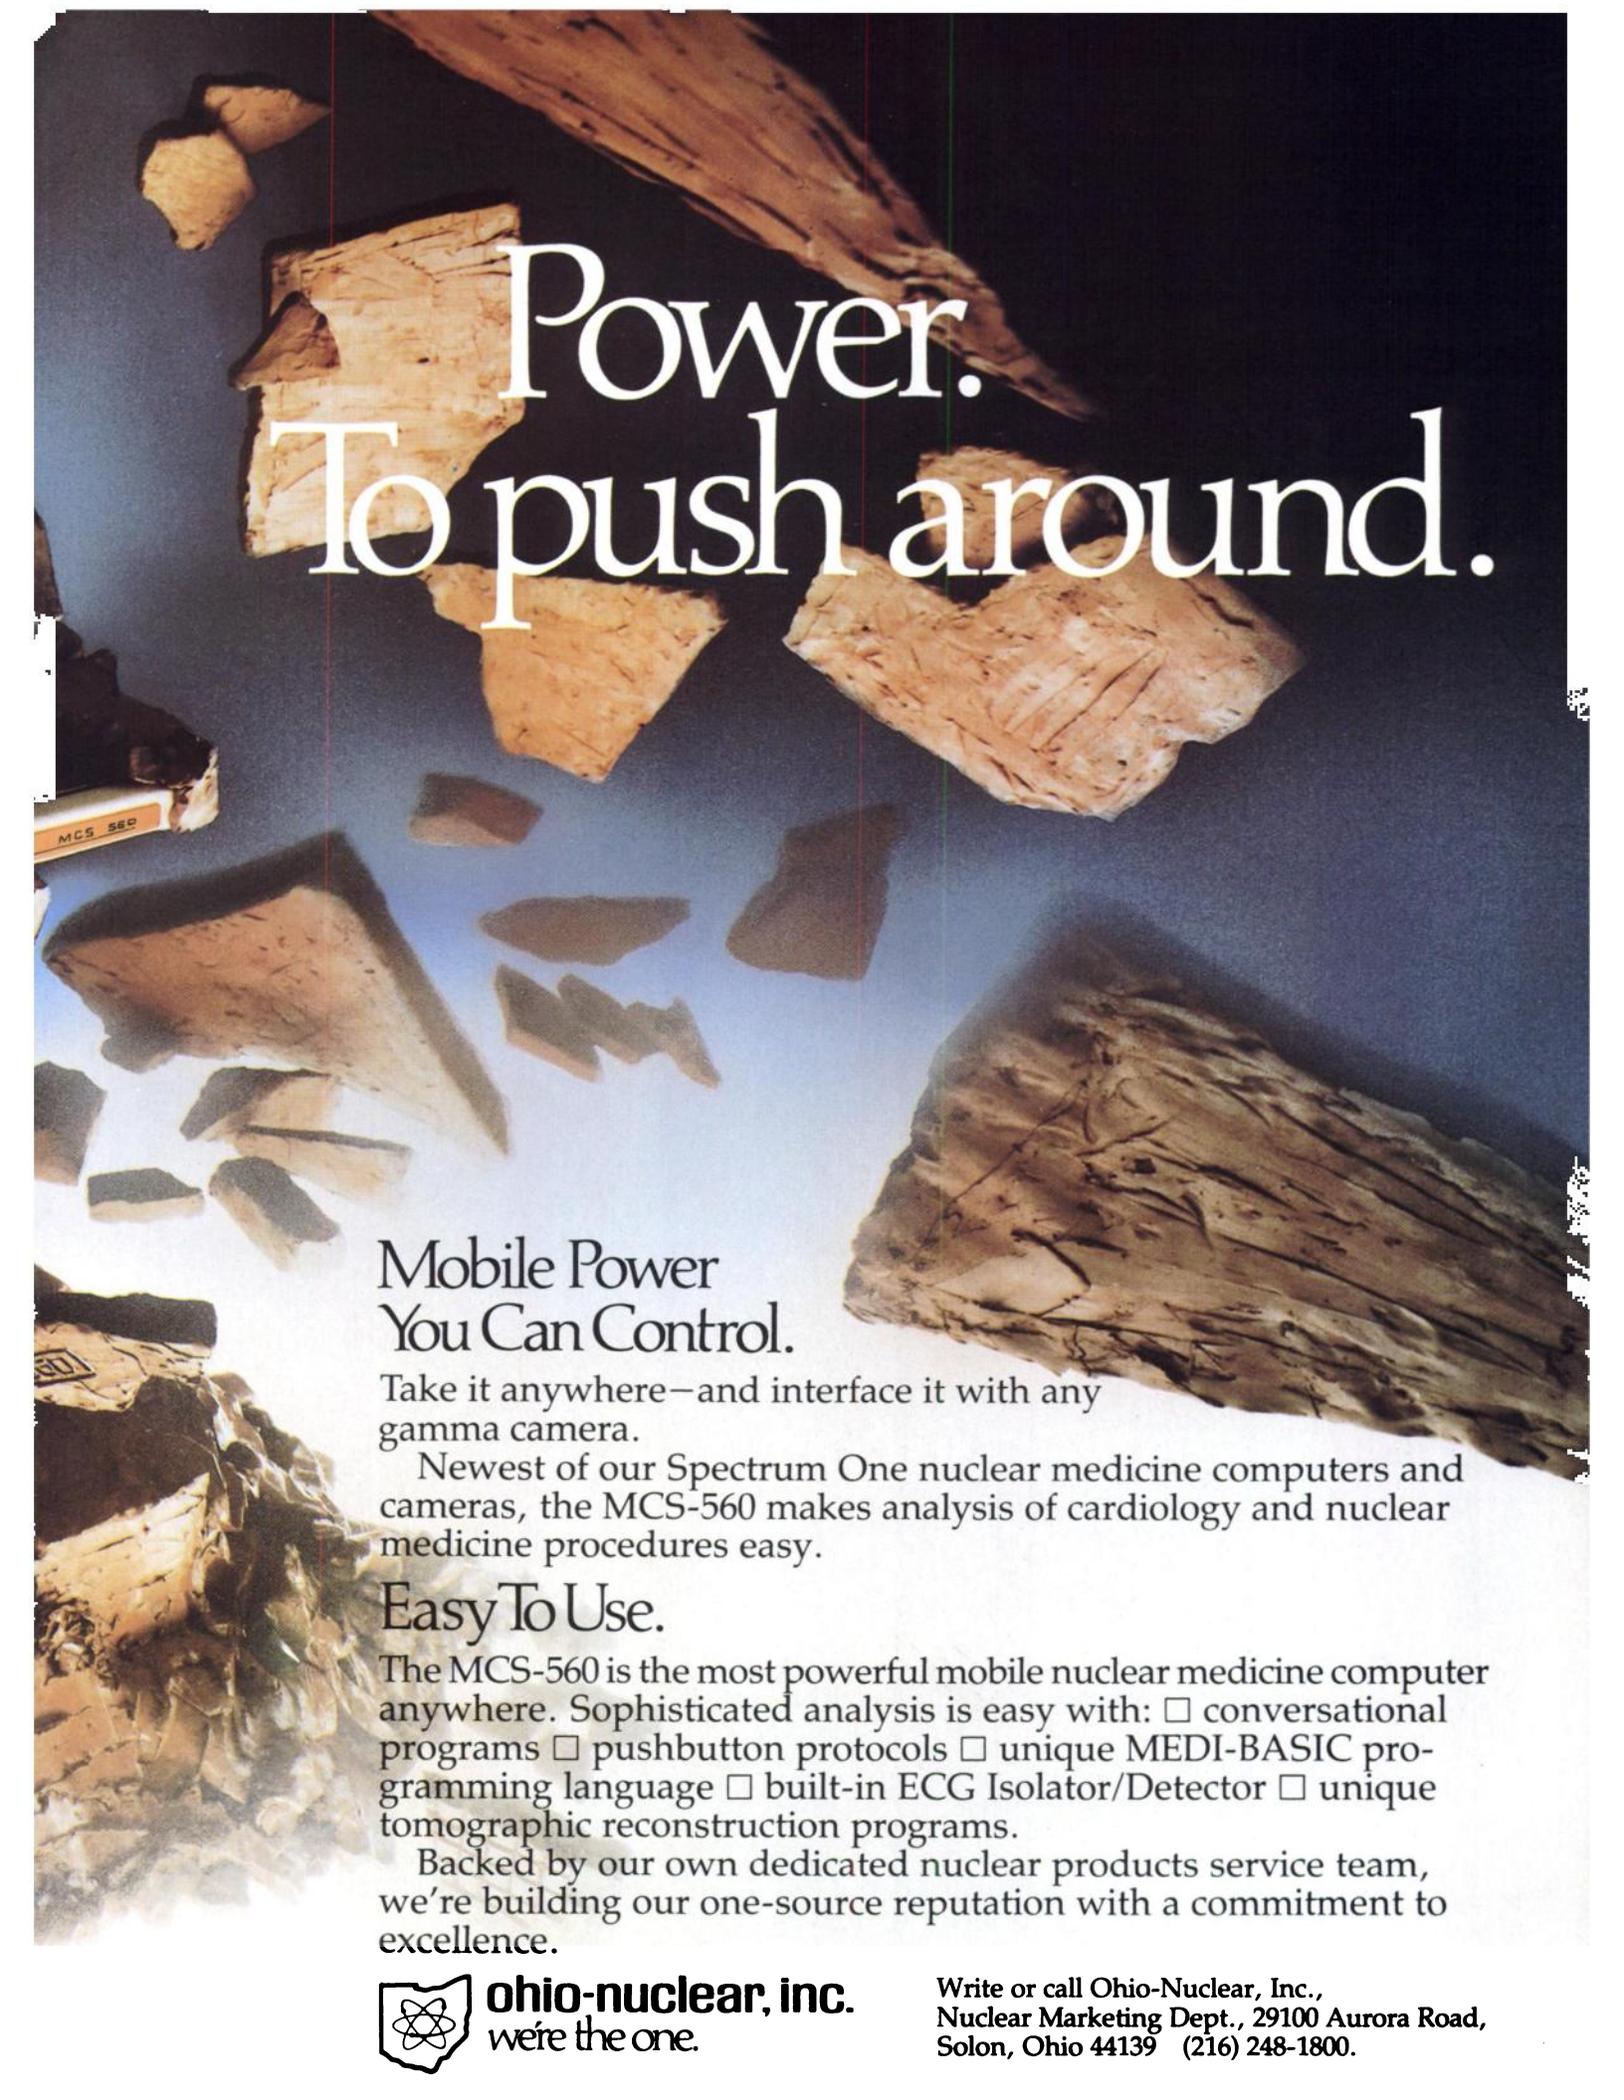

# Power. To push around.

## Mobile Power You Can Control.


Take it anywhere—and interface it with any gamma camera.

Newest of our Spectrum One nuclear medicine computers and cameras, the MCS-560 makes analysis of cardiology and nuclear medicine procedures easy.

## Easy To Use.

The MCS-560 is the most powerful mobile nuclear medicine computer anywhere. Sophisticated analysis is easy with:  conversational programs  pushbutton protocols  unique MEDI-BASIC programming language  built-in ECG Isolator/Detector  unique tomographic reconstruction programs.

Backed by our own dedicated nuclear products service team, we're building our one-source reputation with a commitment to excellence.



**ohio-nuclear, inc.**  
we're the one.

Write or call Ohio-Nuclear, Inc.,  
Nuclear Marketing Dept., 29100 Aurora Road,  
Solon, Ohio 44139 (216) 248-1800.



# **PTH RIA SYSTEM**

**Parathyroid Hormone  
Radioimmunoassay System**

## **ONE (1) DAY ASSAY**

- Precalibrated Standards and Controls
- No Prior Stripping
- Double Antibody Separation
- **Twice The Value**

**Only 24 hours from set up  
to reporting of final results**

**I SO、TEX DIAGNOSTICS**

P. O. Box 909 • FRIENDSWOOD, TEXAS 77546

713/482-1231

# DYCOMETTE

THE COST-EFFECTIVE CLINICAL PROCESSOR  
DESIGNED FOR YOU



- DYCOMETTE offers you the greatest processing capability available today, for your dollar.
  - DYCOMETTE speaks your language — functional keys eliminate need for complex computer codes. So simple, anyone can learn to operate it in hours.
  - High data capacity, fast access time, simple filing, ample storage on floppy disks.
  - Total built-in capability for radiocardiology, including multigated studies at up to 48 frames per cycle, first pass studies, calculation of ejection fraction, cardiac output, shunts and other parameters of major clinical significance.
  - Clinical programs for lung, brain, kidney and other studies.
  - Ability to learn your most frequent procedures and perform them any time later upon command.
  - Full 16 color and 64 gray scale display.
  - Hard copies — on X-ray film and color prints.
  - Compatible with all makes of Gamma Camera.
- If you are cost-effective minded, let us show you what DYCOMETTE can do.  
Call or write today for demonstration or full information.


elscint

The ELSCINT commitment to excellence

**U.S.A.** ELSCINT INC. 138-160 Johnson Avenue, Hackensack, New Jersey 07602, Tel. : 201-487-5885 ; Telex : 135382.  
**Germany** : Elscint GmbH, Freudenbergstrasse 27, 62 Wiesbaden-Schierstein. **U.K.** : Elscint (GB) Ltd. 5 Priestley Way, Crawley, Sussex RH10 2DW.  
**Belgium** : Elscint N.V./S.A. Rue du Saphir 31, B-1040 Brussels. **Holland** : Elscint B.V. Raadhuislaan 12B, Maarn. **Brazil** : Elscint, Rua Dos Moras, 576 Alto De Pinheiros, 05434 Sao Paulo. **Italy** : Elscint S.R.L., Via F. Lli Zoia 75, 20152, Milano. **Israel** : Elscint Ltd., P.O.Box 5258, Haifa.  
**In other countries** — write to: Elscint International Sales & Service Division, Elscint - I.S.S.D., Annandale, North End Road, Golders Green, London NW 11 7QY. **U.K.**

## CMS SCINTISLICE™ TOMOGRAPHY

Multiple, simultaneous imaging.

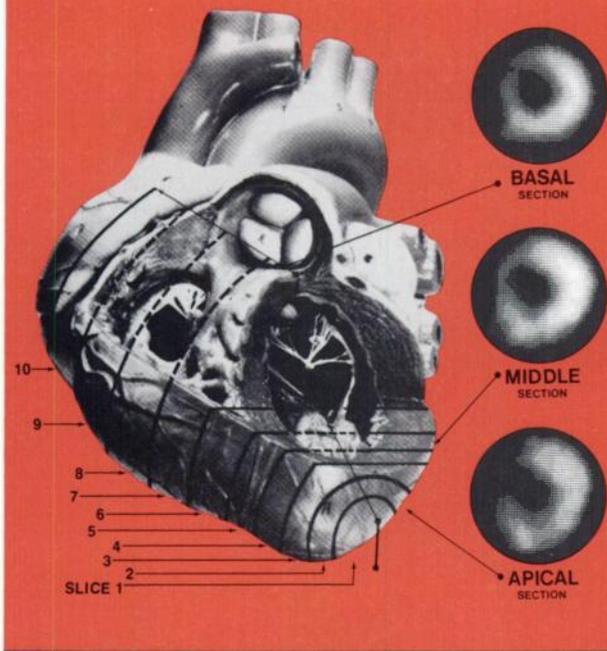

### CMS PROVIDES

Software, Hardware and Installation.

- PROVEN AND VERIFIED PROGRAMS FOR
  - G.E. MED-SERIES
  - DEC GAMMA II
  - INFORMATEK
  - MDS MODUMED
  - MDS A SQUARED
  - ADAC
- LARGE and SMALL FIELD 7 PINHOLE PANORAMIC COLLIMATORS
- GOLD 195 SOURCES and PHANTOM
- ON SITE INSTALLATION and TRAINING

### CMS BILATERAL COLLIMATOR

Multiple, simultaneous imaging.

BILATERAL COLLIMATORS (WITH ROTATION)  
for large and small field Anger cameras  
BILATERAL AND SLANT COLLIMATORS  
for the Cordis / Baird System 77.

# CMS

**WRITE FOR LITERATURE**

**Cardiac Medical Systems Corporation**  
3710 Commercial Avenue, Northbrook, Illinois 60062  
Telephone (312) 564-4644

# The Complete Stress System



## For Any Camera

If you have a nuclear camera, we have the stress system for it. Our HI-LO Stress System allows you to position the pedal ergometer above or below table level so you can use any imaging — even large-field-of-view cameras — while continuously stressing the patient.

The HI-LO Stress System is complete. More than just a table and pedaling unit, our electronic control console features digital displays of Actual Workload, Heart Rate, Pedal Speed, and Elapsed Time. An optional heart rate control allows you to preset and maintain a patient's heart rate and workload.

The mobile control console provides maximum visibility to the operator, and the rugged table can be used for either anterior or posterior imaging. The HI-LO Table is adjustable for supine or seated patient positioning with a separate pedal speed indicator for the patient.


Get the complete story on the only complete Stress System available. Write for more information today.



edc/Medical Imaging  
120 Stedman Street  
Lowell, MA 01851  
617-458-1456

# The Heart—

An advance from Mallinckrodt provides an excellent adjunct in the detection of myocardial infarction and the dynamic assessment of cardiac function.

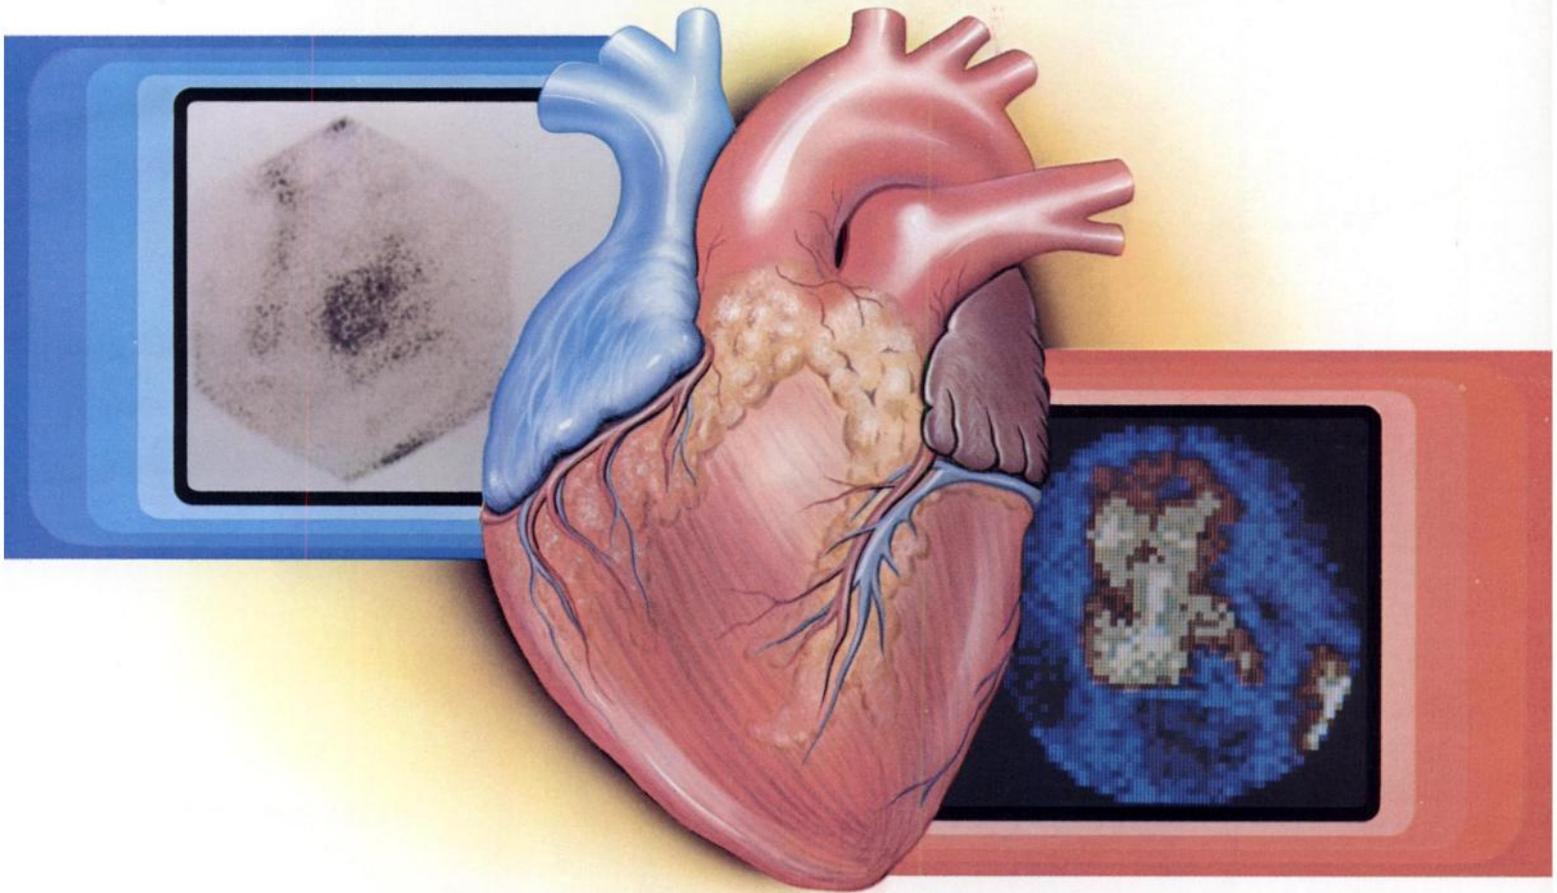

## TechneScan® PYP™ Kit (Stannous Pyrophosphate) for preparation of Technetium Tc-99m Stannous Pyrophosphate.

A consistent agent for skeletal imaging, *TechneScan PYP* is now available for use as an adjunct in the diagnosis of acute myocardial infarction, and for gated cardiac blood-pool imaging.

Investigators have found the technetium-99m pyrophosphate scintigraphic study to be a highly useful diagnostic technique for evaluating chest pain of uncertain origin.<sup>1</sup>

"The gated cardiac blood pool scan permits the calculation of both ejection and regional wall motion from a single examination."<sup>2</sup>

Mallinckrodt's *TechneScan PYP*... a preferred way to detect acute myocardial infarction... an advanced method to dynamically assess cardiac function.

#### References:



1. Berman, DS, et al: New Approach to Interpretation of Technetium-99m Pyrophosphate Scintigraphy in Detection of Acute Myocardial Infarction: Clinical Assessment of Diagnostic Accuracy. *Am. J. Cardiol.* 39:341-346, (March) 1977.
2. Strauss, HW, Pitt, B: Cardiovascular Nuclear Medicine: Its Role in Patients with Coronary Heart Disease. *CVP Journal*: (November/December), 1974.



Mallinckrodt, Inc.  
P.O. Box 5840, St. Louis, Missouri 63134

See reverse side for brief summary of complete prescribing information.

# An advance from Mallinckrodt provides an excellent adjunct in the detection of myocardial infarction and the dynamic assessment of cardiac function.

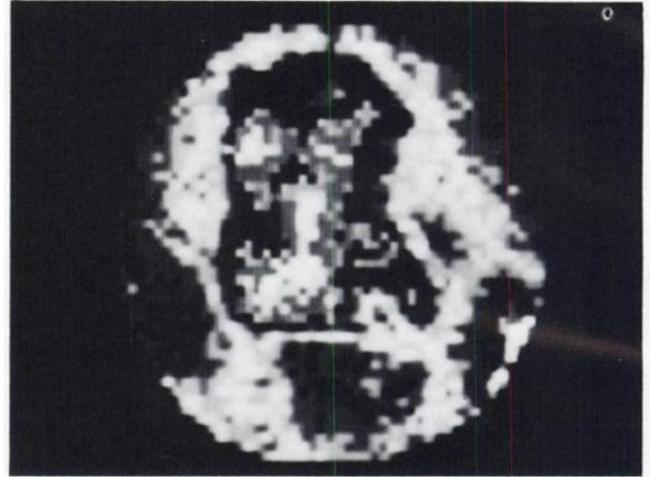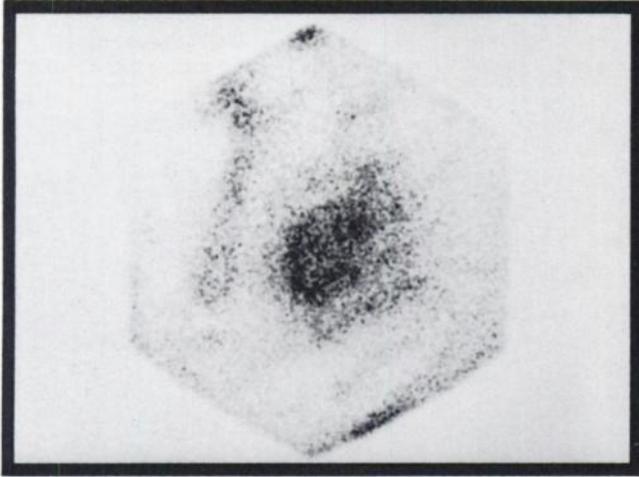

## TechneScan® PYP™ Kit (Stannous Pyrophosphate) for preparation of Technetium Tc-99m Stannous Pyrophosphate.

### BRIEF SUMMARY

#### CLINICAL PHARMACOLOGY

When injected intravenously **TechneScan PYP Tc 99m** has a specific affinity for areas of altered osteogenesis. It is also concentrated in the injured myocardium, primarily in areas of irreversibly damaged myocardial cells.

One to two hours after intravenous injection of **TechneScan PYP Tc 99m**, an estimated 40 to 50 percent of the injected dose has been taken up by the skeleton and approximately 0.01 to 0.02 percent per gram of acutely infarcted myocardium. Within a period of one hour, 10 to 11 percent remains in the vascular system, declining to approximately 2 to 3 percent twenty-four hours post injection. The average urinary excretion was observed to be about 40 percent of the administered dose after 24 hours.

**TechneScan PYP** also has an affinity for red blood cells. When administered 30 minutes prior to the intravenous administration of sodium pertechnetate Tc-99m approximately 76 percent of the injected activity remains in the blood pool providing excellent images of the cardiac chambers.

#### INDICATIONS AND USAGE

**TechneScan PYP Tc 99m** is a skeletal imaging agent used to demonstrate areas of altered osteogenesis, and a cardiac imaging agent used as an adjunct in the diagnosis of acute myocardial infarction.

As an adjunct in the diagnosis of confirmed myocardial infarction (ECG and serum enzymes positive), the incidence of false negative images has been found to be 6 percent. False negative images can also occur if made too early in the evolutionary phase of the infarct or too late in the resolution phase. In a limited study involving 22 patients in whom the ECG was positive and serum enzymes questionable or negative, but in whom the final diagnosis of acute myocardial infarction was made, the incidence of false negative images was 23 percent. The incidence of false positive images has been found to be 7 to 9 percent. False positive images have also been reported following coronary by-pass graft surgery, in unstable angina pectoris, old myocardial infarcts and in cardiac contusions.

**TechneScan PYP** is a blood pool imaging agent which may be used for gated cardiac blood pool imaging. When administered intravenously 30 minutes prior to the intravenous administration of sodium pertechnetate Tc-99m approximately 76 percent of the injected activity remains in the blood pool.

#### CONTRAINDICATIONS

None.

#### WARNINGS

This radiopharmaceutical should not be administered to patients who are pregnant or lactating unless the information to be gained outweighs the potential hazards.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

**Warning:** Preliminary reports indicate impairment of brain scans using pertechnetate Tc-99m which have been preceded by bone scan. The impairment may result in false positives or false negatives. It is recommended, where feasible, that brain scans precede bone imaging procedures.

Radiopharmaceuticals should be used only by physicians who are qualified by specific training in the safe use and handling of radionuclides produced by nuclear reactor or particle accelerator and whose experience and training have been approved by the appropriate government agency authorized to license the use of radionuclides.

The **TechneScan PYP** Kit must be maintained at refrigerator temperature until use.

The contents of the **TechneScan PYP** reaction vial are intended for use in the preparation of Technetium Tc 99m Stannous Pyrophosphate. **TechneScan PYP** may also be

reconstituted with sterile, pyrogen-free normal saline containing no preservatives and injected intravenously prior to the administration of sodium pertechnetate Tc-99m.

Sodium pertechnetate Tc-99m solutions containing an oxidizing agent are not suitable for use with the **TechneScan PYP** Kit.

The contents of the kit are not radioactive. However, after the sodium pertechnetate Tc-99m is added, adequate shielding of the final preparation must be maintained.

**TechneScan PYP Tc 99m** should not be used more than six hours after preparation.

#### PRECAUTIONS

As in the use of any other radioactive material, care should be taken to insure minimum radiation exposure to the patient, consistent with proper patient management, and to insure minimum radiation exposure to occupational workers.

#### Bone Imaging

Both prior to and following **TechneScan PYP Tc 99m** administration, patients should be encouraged to drink fluids. Patients should void as often as possible after the **TechneScan PYP Tc 99m** injection to minimize background interference from accumulation in the bladder and unnecessary exposure to radiation.

#### Cardiac Imaging

Patient's cardiac condition should be stable before beginning the cardiac imaging procedure.

If not contraindicated by the cardiac status, patients should be encouraged to ingest fluids and to void frequently in order to reduce unnecessary radiation exposure.

Interference from chest wall lesions such as breast tumors and healing rib fractures can be minimized by employing the three recommended projections.

#### Blood Pool Imaging

**TechneScan PYP** should be injected by direct venipuncture. Heparinized catheter systems should be avoided.

#### ADVERSE REACTIONS

None.

#### HOW SUPPLIED

Catalog Number—094 **TechneScan PYP Kit**

#### Kit Contains:

5—Stannous Pyrophosphate Reaction Vials (lyophilized) for the preparation of Technetium Tc-99m Stannous Pyrophosphate.

#### Reaction Vial Contains:



12.0 mg sodium pyrophosphate and 3.4 mg stannous chloride (lyophilized). Hydrochloric acid is added for pH adjustment prior to lyophilization.

5—Radioassay Information String Tags.



Mallinckrodt, Inc.  
P.O. Box 5840, St. Louis, Missouri 63134

# Matrix video cameras do everything but develop the film... and that's next.

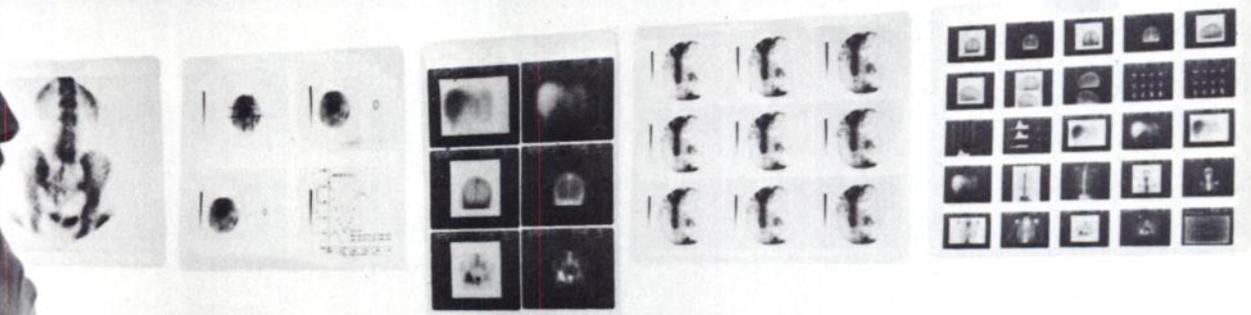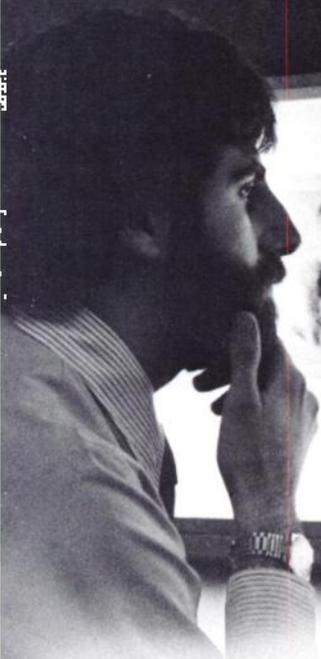

Everything medical imaging cameras should do, that is. Effortlessly. Automatically. Excellently, in over 1,000 new installations a year. Matrix video cameras embody the latest in video, optical and microprocessor technology. They handle the relatively diverse demands of ultrasound and nuclear computers as well as the special, high line rate requirements of CT or fluoroscopy reproduction. They give you quality images, from which you can diagnose confidently.

The video cameras that do everything are *the only ones which automatically adjust exposure time*. Other camera systems make you do it manually. We think you have enough to do. Matrix cameras have a photometer which measures a calibration pattern. *Before each exposure*, it reads light levels, compares them with optimum values and adjusts accordingly. Automatically. All in a quarter of a second. You can be confident the scans you do at the end of the day will have the same gray scale content as the ones you do at the beginning of the day.

The "do-everything" cameras have the widest selection of image size formats to meet the needs of your lab or service. With the Multi-Imager 7 as many as 8 different ones. With the Video Imager, as few as one. Flexibility from a single large image to 25 slide size images. Film sizes of 8"x10" and 11"x14". All from one camera!

Most of all, you get excellent, effortless diagnostic images, automatically. Nothing less than you'd expect from the camera that does everything but develop the film... AND THAT'S NEXT, FROM MATRIX.

## ✱ MATRIX INSTRUMENTS

230 Pegasus Ave., Northvale, N.J. 07647  
(201) 767-1750 Toll Free: (800) 526-0274  
Telex: 135131

Worldwide sales and service.  
Contact international department.



Please send more information and sample studies. JNM

- |  |  |
|--|--|
| <input type="checkbox"/> Ultrasound                    | <input type="checkbox"/> Nuclear Medicine Computer |
| <input type="checkbox"/> CT                            | <input type="checkbox"/> Fluoroscopy               |
| <input type="checkbox"/> Nuclear Medicine Gamma Camera |  |

Name \_\_\_\_\_ Title \_\_\_\_\_

Hospital \_\_\_\_\_ Dept. \_\_\_\_\_

Address \_\_\_\_\_

City \_\_\_\_\_ State \_\_\_\_\_ Zip \_\_\_\_\_



# Tech It!

**Because quality is important to your image ... Check your Products with a Tech Kit! It's the only move to make.**

Tech is a quality control testing system which provides a quick, convenient and inexpensive means for determining unbound and free Technetium 99m in the following products:

PYROPHOSPHATE  
DIPHOSPHONATE  
POLYPHOSPHATE  
MDP

PHYTATE  
DTPA  
MICROSPHERES  
HUMAN SERUM ALBUMIN

GLUCOHEPTONATE  
SULFUR COLLOID  
MACROAGGREGATED ALBUMIN

For more detailed information, contact:



**ACKERMAN NUCLEAR, INC.**

*Pharmaceuticals for Nuclear Medicine*  
445 West Garfield Avenue  
Glendale, California 91204, U.S.A.  
(213) 246-2555



# Back to Basics!

## The Assayer 1 by Radx

The never ending struggle for product popularity often leads a manufacturer to add gadgets. It's called "one-upmanship." We sometimes lose sight of what YOU, the user, wants.

By customer demand, Radx has gone "Back to Basics" and developed the Assayer 1, a simple dose calibrator, a reliable dose calibrator, an economical dose calibrator.

The return to basics does not require a

return to the 1960's technology. The Assayer 1 is microprocessor controlled, totally solid state, with a method of isotope selection way ahead of its time (an optical scanner) which is so precise, reproducible, and reliable that it will soon be copied.

It is not a gadget, it calibrates doses accurately, with precision and unprecedented reliability. It's the Assayer 1—\$2950.

Call today for the last dose calibrator you'll ever own.

**RADIX**


P.O. Box 19164 • Houston, Texas 77024 • (713) 468-9628

# R WAVE GENERATOR

FOR  
NUCLEAR CARDIOLOGY

## BEHIND EVERY SQUARE WAVE THERE IS AN R WAVE

If all you need is a square wave to trigger the computer every time an R wave occurs then talk to us before you make a decision. We can provide you with a reliable system and save you money. Why buy unnecessary features that cost you extra? Our R wave generator provides only the features that you need.

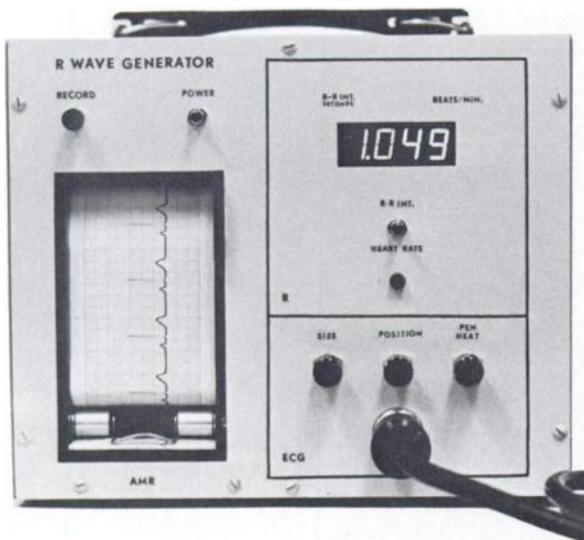

### INSTRUMENT HIGHLIGHTS

- Compact and inexpensive unit which records ECG on strip chart for permanent record.
- Four digit LED display to indicate R-R interval in seconds or heart rate in beats per minute. The R-R interval display is used to decide the gate tolerance. The heart rate display is helpful during stress testing.
- Produces sharp square wave output for R wave which can be used as a trigger for nuclear cardiology applications.


Delivery is 90 Days or less depending upon stock.

For price information call: (203) 877-1610 or write to:

**Customer Service, AMR CORP., P. O. Box 3094 PPS, Milford, Conn. 06460**

## Nuclear Medicine Modular Systems

Kewaunee Nuclear Medicine Modular Systems consist of lead shielded modules specifically designed with a "Work-Flow" pattern for Receiving, Holding and Storage, Reagent Preparation, Inventory and Dispensing of Radiopharmaceuticals and Decay Storage.

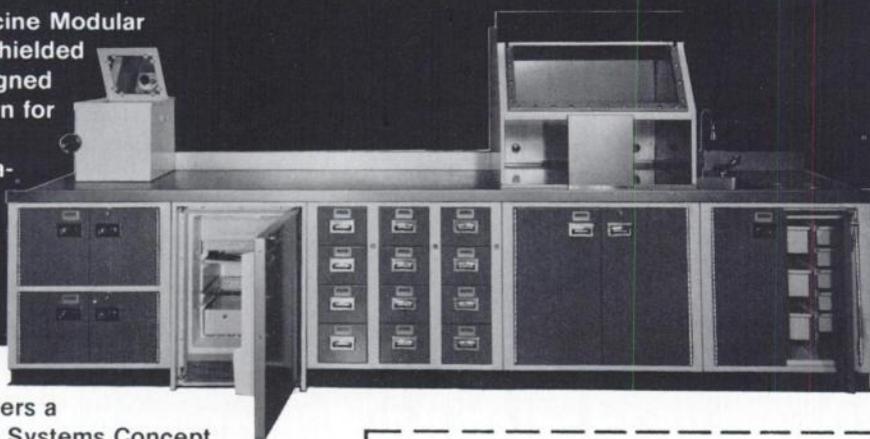

The Kewaunee design offers a complete Radiopharmacy Systems Concept for Nuclear Medicine Departments. Lead shielding within the system provides for personnel safety from radiation. Maximum efficiency is obtained through the "Work-Flow" pattern concept.



**kewaunee**

**KEWAUNEE SCIENTIFIC EQUIPMENT CORP.**  
Special Products Division  
Lockhart, Texas 78644  
Phone: 512/398-5294

- Please send literature  
 Please have representative call.

Name \_\_\_\_\_ Title \_\_\_\_\_

Organization \_\_\_\_\_


Address \_\_\_\_\_

City \_\_\_\_\_ State \_\_\_\_\_ Zip \_\_\_\_\_

Phone \_\_\_\_\_

# Look at this

## a cardiac stress system that does more and costs less

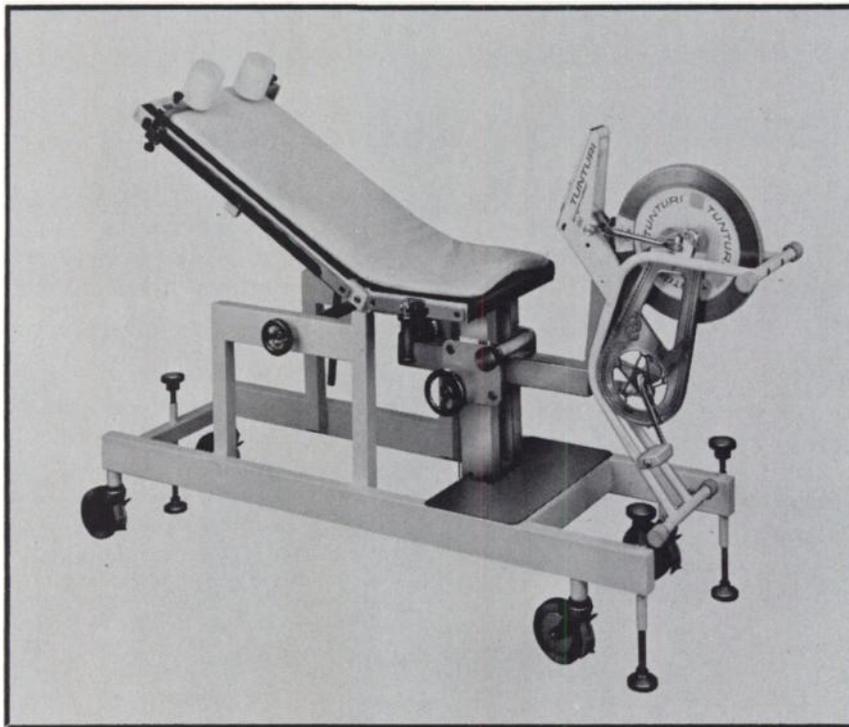

Model  
056-180

### DESIGNED FOR EXERCISE IMAGING

- Allows variable patient positioning at any angle from supine to upright.
- Ergometer positions are easily adjusted vertically and horizontally to accommodate any patient physique and study orientation.
- Designed for use with all large field of view cameras and for oblique views.
- Wheel and floor lock design to avoid camera pedestal interference and to provide positive table rigidity.
- Contoured seat and back provide patient comfort and positive restraint. Eliminates unnatural reach and strain.
- Straps, hand grips, shoulder pads hold patient firmly in position.
- Table can be used with most commercially available ergometers.

FOR COMPLETE INFORMATION WRITE OR CALL—

### Atomic Products Corporation

ATOMLAB DIVISION • ESTABLISHED 1949  
P.O. BOX 657 CENTER MORICHES, NEW YORK 11934 USA  
(516) 878-1074  
TWX #510-228-0449

# COLLEGE OF AMERICAN PATHOLOGISTS

presents a



ENDORSED BY  
AMERICAN COLLEGE  
OF RADIOLOGY

# NUCLEAR MEDICINE PROGRAM

in 1980



ENDORSED BY  
SOCIETY OF  
NUCLEAR MEDICINE

## TRANSMISSION IMAGING SIMULATOR SERIES X

PRICE **\$367.00**

SHIPMENTS: **X•A/May**      **X•B/October**

Each of two shipments will contain an unknown imaging device permitting.

- Inter-laboratory comparison of technique and instrumentation.
- Initiation and maintenance of a continuing quality control program of imaging procedures.

Summary reports with extensive educational critiques provide participants with opportunities for sharing state of the art information regarding equipment, methods, and techniques.

Due to the success of the imaging simulator (phantom) in 1979, and its planned implemented use in 1980, it is no longer necessary to obtain an amendment by those applicants having licenses from the N.R.C., since it no longer contains radionuclides.

The CAP cannot guarantee that all shipments in a series will be available for orders received after December 31, 1979. There is an administrative charge of \$20 for orders receiving partial shipments.

## NUCLEAR MEDICINE SPECIAL STUDIES RADIONUCLIDE ACTIVITY MEASUREMENT SERIES Q

PRICE **\$302.00**

SHIPMENTS: **Q•A/April**      **Q•B/October**

*Series Q is designed to provide:*

- An accuracy assessment of radioactivity assay procedures
- An evaluation of procedures for determination of radionuclidic purity
- An intercomparison of results between laboratories
- An opportunity to establish calibration factors for instruments

Each of two shipments will contain a sample certified by the National Bureau of Standards for identity, purity, and activity. Participants will identify the nuclide by pulse-height analysis and measure its activity with instruments available in their laboratory. The samples may be retained for use as a certified standard.

**NOTE:** An amendment must be obtained by those applicants having licenses from N.R.C. (except Broad Medical) and Agreement states (except Broad Medical) to obtain radionuclides for calibration purposes.

----- PLEASE TYPE OR PRINT—FILL IN AND MAIL FORM TO: -----

## COLLEGE OF AMERICAN PATHOLOGISTS / 7400 NORTH SKOKIE BLVD. / SKOKIE, IL 60077 CAP / 1980 NUCLEAR MEDICINE PROGRAM

PLEASE SEND:      EXTENDED COST

<input type="checkbox"/> Sets of <b>Series X</b> @ <b>\$367</b> per set	
<input type="checkbox"/> Sets of <b>Series Q</b> @ <b>\$302</b> per set	
Total Amount	
Prepaid Amount	
Total Due	

AUTHORIZED SIGNATURE: (Required for Processing)

Check below to have Evaluation Copies sent to the following:

- Participation in these programs is to meet state and/or Medicare proficiency testing requirements. Copies of test results are to be sent to the state agency:

STATE \_\_\_\_\_ I.D. NUMBER \_\_\_\_\_

Check or Purchase Order must accompany subscription—payable to:  
COLLEGE OF AMERICAN PATHOLOGISTS

P.O. # \_\_\_\_\_ Enclosed

For CAP Office use only:

Batch No. \_\_\_\_\_ 19

CAP No. (If Applicable)  •

**Send Survey Sets to:** PLEASE TYPE OR PRINT

NAME \_\_\_\_\_  
INSTITUTION \_\_\_\_\_  
ADDRESS \_\_\_\_\_  
CITY \_\_\_\_\_ STATE \_\_\_\_\_ ZIP \_\_\_\_\_  
JNM-12

**Bill to:**


NAME \_\_\_\_\_  
INSTITUTION \_\_\_\_\_  
ADDRESS \_\_\_\_\_  
CITY \_\_\_\_\_ STATE \_\_\_\_\_ ZIP \_\_\_\_\_

# ATTENTION DEC GAMMA 11™ OWNERS:

**Your Gamma-11 can now produce high-quality, 3-dimensional, 7-pinhole emission tomography in 60 seconds!**

We call it the **GAMMECAT™ Package**.

You only need our GAMMECAT system, your computer and most Anger cameras.

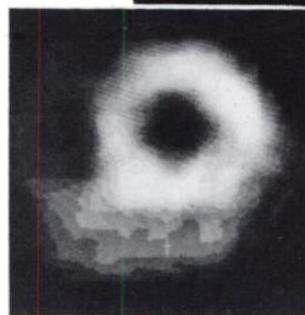

One plane through myocardium parallel to collimator.

The GAMMECAT Package was developed by the pioneers of 7-pinhole tomography. It features the fastest and most accurate software available today. We combined the technology of 7-pinhole tomography with the advances of GAMMECAT software.

Consider the following:

- 7-pinhole tomography - increases sensitivity without any loss of specificity in thallium myocardial perfusion studies.<sup>1,2</sup>
- images the heart in true-to-life 3 dimensions.
- saves valuable camera time by shooting multiple views simultaneously.

- GAMMECAT offers - speed, by reconstructing multiple images into 10 planes in 60 seconds.
- accuracy, through state of the art linear reconstructions, with minimal artifacts.
- constant plane thicknesses with automatic correction for pinhole magnification.
- a complete system, including a collimator, and everything needed for 7-pinhole tomography.
- economy and simplicity, by utilizing your existing camera and computer system.

..... In a word,  
7-pinhole tomography is a breakthrough;  
GAMMECAT is the most advanced application package available.



## RESEARCH SYSTEMS, INC.

2021 Albion Street,  
Denver, Colorado 80207  
Telephone (303) 399-1326


<sup>1</sup>Vogel RA, Kirch DL, Lefree MT, Rainwater JO, Steele PP: Thallium-201 myocardial perfusion scintigraphy: Results of standard and multi-pinhole tomographic techniques. *The American Journal of Cardiology* 43:787-793, 1979

<sup>2</sup>Francisco D, Raymundo G, Van Kirk O, Erhardt J, Marcus M: Tomographic thallium-201 perfusion scintigrams following maximal coronary vasodilation with dipyridamole: Circulation (in press)


\*DEC Gamma 11 is a trademark of Digital Equipment Corporation

**WATCH FOR OUR REVOLUTIONARY TOMOGRAPHIC GATED CARDIAC ANALYSIS PACKAGE**

Birdcage representation of the surface of the blood pool inside the left ventricle.




This package, in conjunction with 128 by 128 gated acquisition software, will present the left ventricular blood pool as it actually appears, in 4 dimensions (3 spatial, plus time). Only one LAO gated tomographic study is needed to view the beating blood pool from any desired angle.



Computer simulation of blood pool.

# THE O'NEILL STRESS SYSTEM

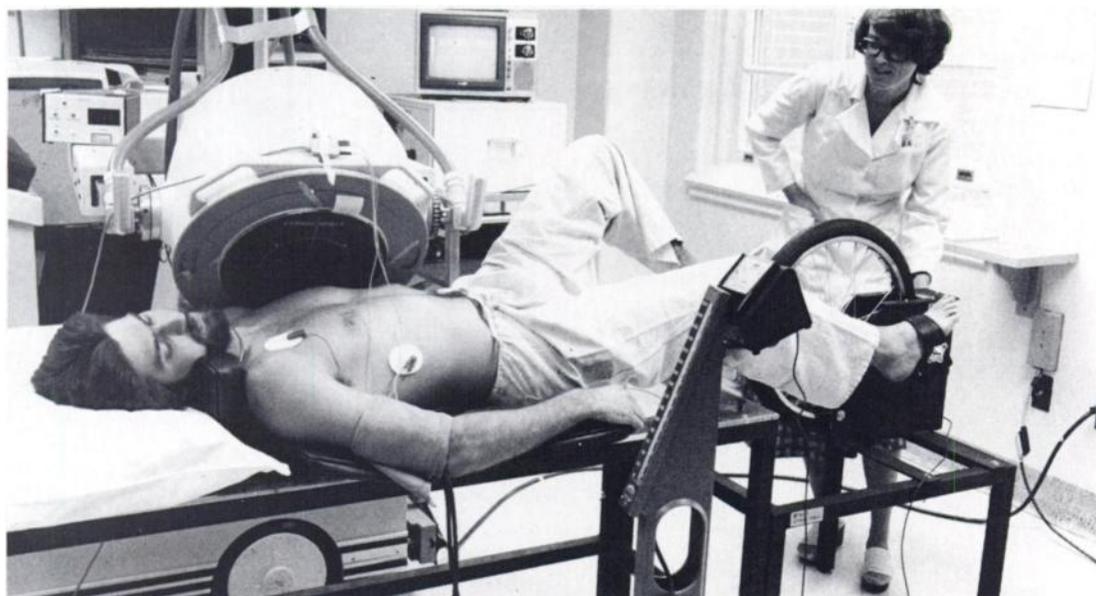

**...DESIGNED EXPRESSLY FOR NUCLEAR CARDIOLOGY**  
**...DESIGNED FOR HEAVY DUTY TROUBLE-FREE USE!**  
**...DESIGNED FOR THE COST-CONSCIOUS BUYER!**

O'NEILL ENTERPRISES 221 FELCH ST. ANN ARBOR MICHIGAN 48103 (313) 973-2335

## JUST PUBLISHED!

### **Radiopharmaceuticals II: Proceedings of the 2nd International Symposium on Radiopharmaceuticals**

This volume is a complete compilation of papers presented at the Second International Symposium on Radiopharmaceuticals, held March 19-22, 1979, in Seattle, Washington. More than 70 papers in this volume cover the complete spectrum of radiopharmaceuticals: from production through quality control to the latest in radionuclide agents for imaging and other studies.

The 867 page, illustrated volume contains chapters titled: Quality Control; Organic Radiopharmaceuticals; Inorganic Radiopharmaceuticals; Functional Imaging; RIA; Oncology; Hematology; Pharmacokinetics; Renal; Cardiopulmonary System; RES/Biliary; Skeletal; Thyroid; Pancreas, Prostate, and Adrenals; and Radionuclide Production. Also included are papers given in a panel discussion entitled "International Regulatory Affairs Relating to Radiopharmaceuticals," and the Keynote Address by Gov. Dixy Lee Ray.

867 pages. Illustrated. Price \$40.00, plus \$1.00 for postage and handling. Check or purchase order must accompany all orders. (Payment in U.S. funds only.)

Copies are available now. Order from:

**Book Order Dept.  
Society of Nuclear Medicine  
475 Park Avenue South  
New York, NY 10016.**

Medi-Ray announces . . .

# SURVEY METER

## CALIBRATION and REPAIR SERVICE

The Medi-Ray Survey Meter Calibration and Repair Service is designed to provide reliable, competent calibration and repair for the areas of Nuclear Medicine, Radiology, Research and Industry. Our service incorporates the latest techniques and facilities, as well as a staff of highly qualified personnel functioning in the latest and most modern of environments. The result is the highest quality service at a reasonable cost to the customer.

### Types of Meters:


- Ionization Chamber
- Geiger — Mueller
- Scintillation

### Features:

- New York State Licensed Laboratory
- Three calibration points on each range
- Accuracy  $\pm$  10% of indicated reading
- Low cost — \$50.00 meter calibration  
\$50.00 repair service (excluding GM tube replacement)
- Rapid turnaround

For information, write or call collect:


Medi-Ray, Inc. / 150 Marbledale Rd. / Tuckahoe, N.Y. 10707  
(914) 961-8484

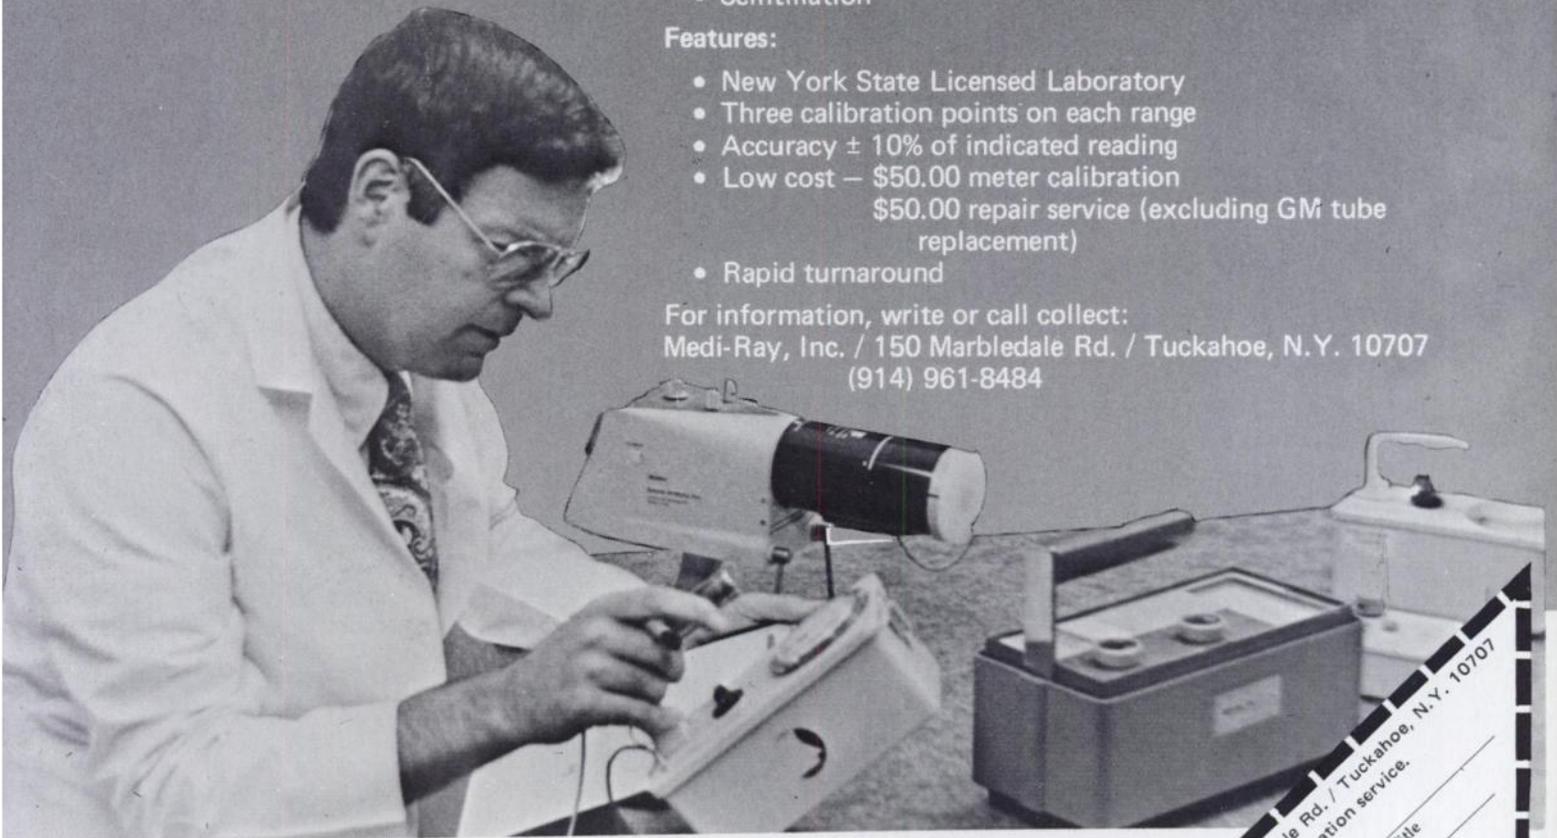

# Medi-Ray, Inc.

Medi-Ray, Inc. / 150 Marbledale Rd. / Tuckahoe, N.Y. 10707  
Please send information on calibration service.

Name	_____
Hospital	_____
Address	_____
State	_____
City	_____
Zip	_____
Phone	_____
Title	_____
Dept.	_____

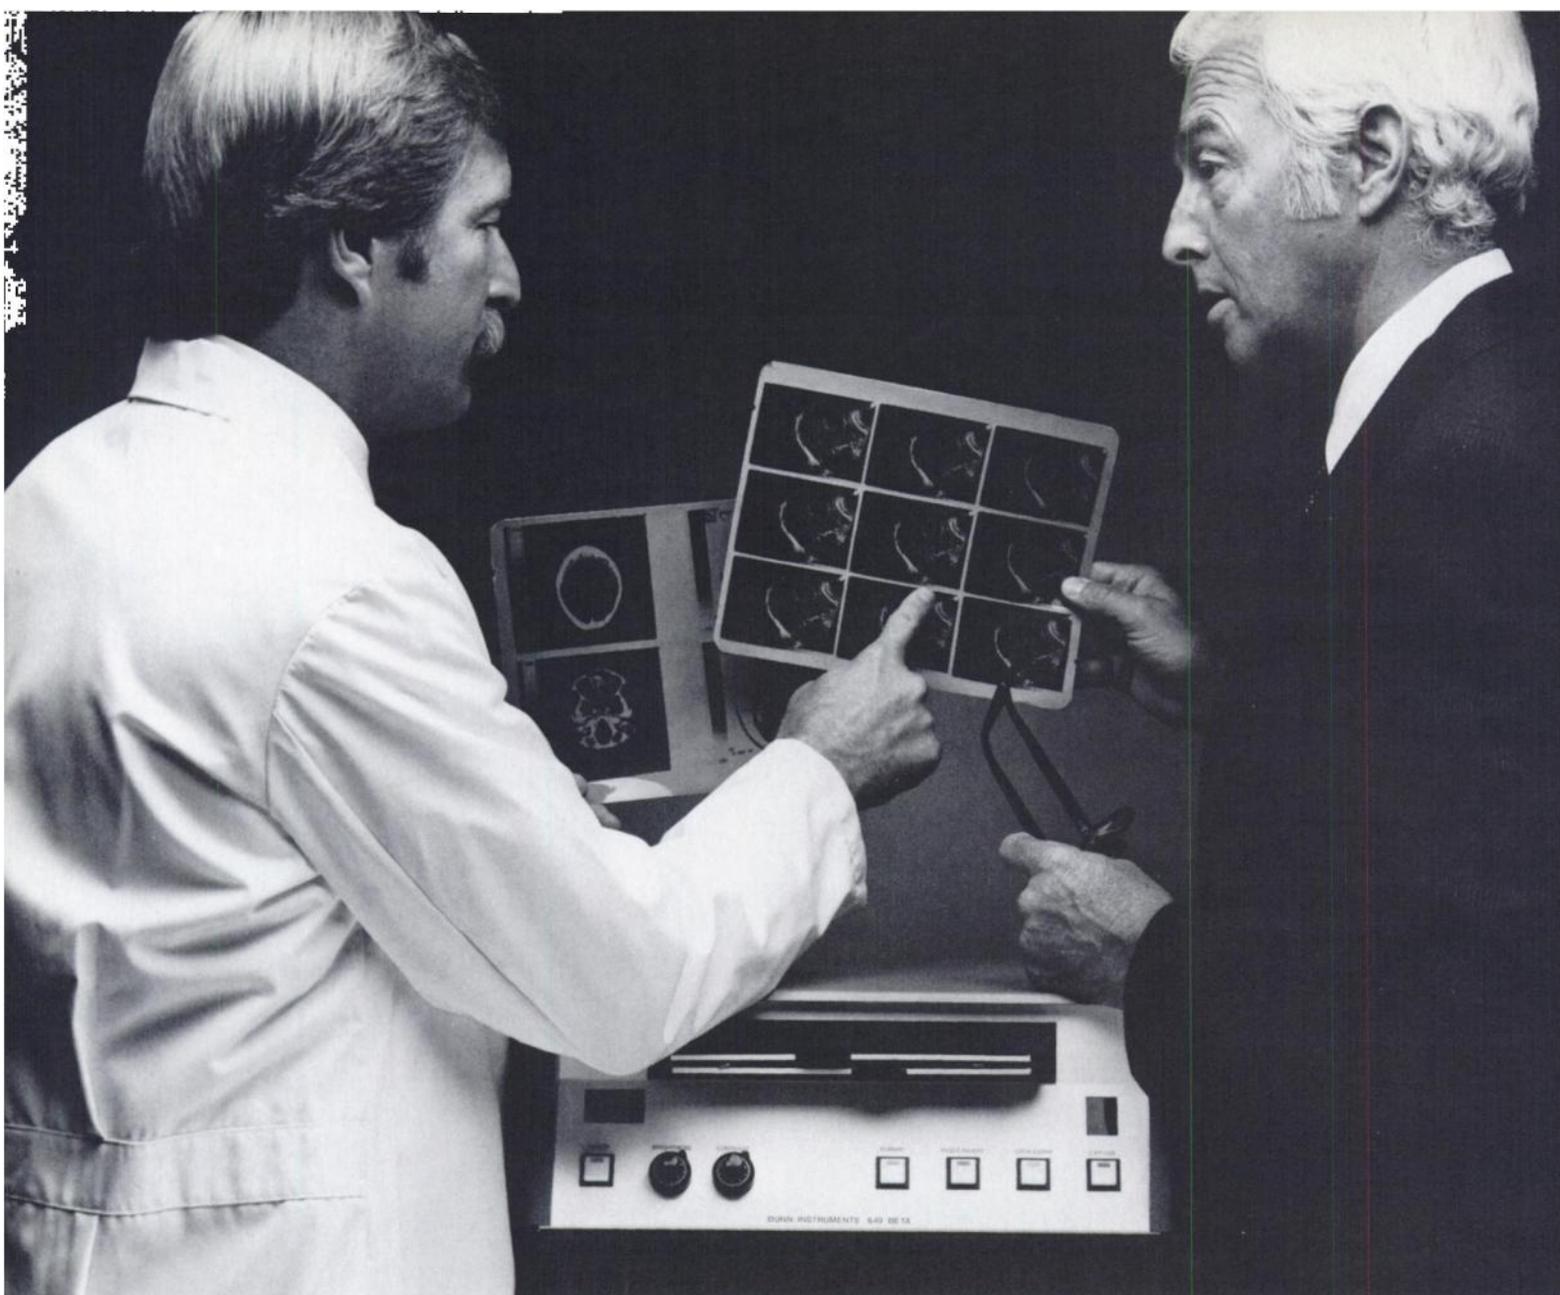

# New Faithful

## The multi-format 649 camera joins the Beta Series.


Faithful rendition of the medical image. And faithful operation at the touch of a button. Dunn's Model 649 has been around long enough to prove its worth. But now it's new again. Why? Because it has been thoroughly re-designed and re-engineered to take its place in the Beta Series. Now the finest series of fixed-format multi-image cameras also offers the advantages of multiple formats where they're needed.

Beta design means effortless and error-proof operation, thanks to

programmable microprocessor electronics. It means a service record to envy. And most important, the superb optical and video components mean perfect pictures every time, in any format.


Whatever your imaging needs, in CT, ultrasound or fluoroscopy, you will want to check out the Beta Series, including the new 649. Find out why the inventors of the multi-image camera still make the best. Call or write for full information and sample films. Dunn Instruments, Inc., 544 Second Street, P.O. Box 77172, San Francisco, CA 94107. Tel. 415/957-1600.

**DUNN  
INSTRUMENTS**  
The precision image

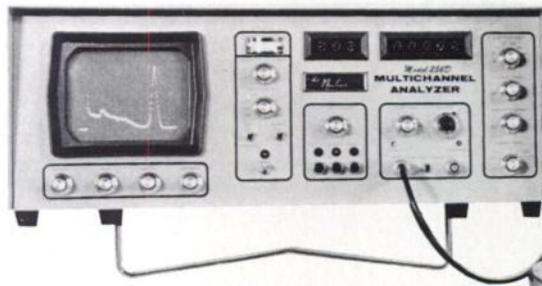

MODEL 256D  
WELL COUNTING SYSTEM

**\$4095 COMPLETE**  
U.S. DOMESTIC

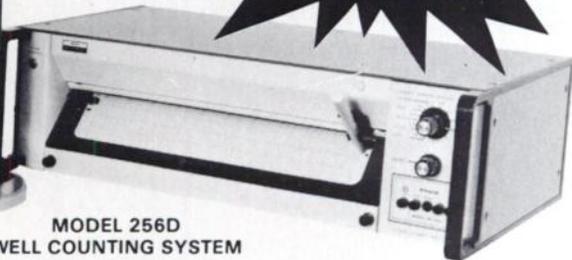

# GAMMA SPECTROMETER for NUCLEAR MEDICINE

Do you check your incoming radionuclides for purity and possible contamination? Better yet, do you have permanent proof of your quality assurance?

With over 20 years of experience in nuclear instrumentation, The Nucleus offers two complete gamma spectrometry systems designed for radionuclide analysis — and at a price suitable for tight budgets!

## MULTICHANNEL ANALYZER



A multichannel analyzer is ideally suited for gamma scintillation spectrometry utilizing a NaI well-type detector. Our standard Model 256D (256 channels of memory) offers all the features required to analyze and compare a known gamma spectra with any unknown sample. And, the data add/subtract feature lets you "strip" known spectra from a mixture of radionuclides. For more sophisticated solid state detectors, we recommend the Model 1024D with 1024 channels of memory. Standard features on the 1024D include an integral 8-decade region of interest sum counter, multichannel scaling, and teletype output. Both models offer a direct reading LED display of channel number and total counts per channel with an illuminated marker cursor.

## SCOPE DISPLAY



The built-in 5-inch CRT provides a bright, clear display of the accumulated data. On the Model 256D, the memory may be split into halves, 128/128 channels each. This permits direct comparison of spectra. For example, store a known I-125 spectrum in the first half, and then examine the second half spectrum of an incoming shipment. The Model 1024D features a 1024 channel memory which may be split into halves and quarters; each may be overlapped for direct comparison. Naturally, both vertical and horizontal expands are standard on every Nucleus MCA.


## WELL DETECTOR




Numerous NaI scintillation probes are available for nearly every gamma spectrum analysis requirement. If you already have such a detector, most likely it will be compatible with either of these multichannel analyzers. Pictured is our Model WP-2000 well-type NaI scintillation probe with a 1.75" by 2" well crystal, on a 2" photomultiplier tube. Well size is .7" (17 mm) diameter by 1.5" (3.8 mm) deep. Resolution is 9% or better, full-width-half-maximum for Cs-137 (0.662 meV). The crystal is surrounded by .75 inches of lead.

## HARD COPY RECORDER

For permanent records, a hard copy recorder documents the accumulated spectra. Any chart recorder is compatible, and several inexpensive models are available. Of course, a scope camera by Polaroid makes quick work of documentation. Linear and log readouts are standard features of these MCAs. Reproduced below are actual copies or photographs of some gamma spectra.



HARD COPY RECORD

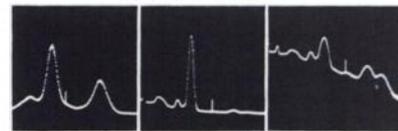

SCOPE DISPLAYS

## AVAILABLE NOW!

Picture what a Nucleus Gamma Spectrometer can do in your lab. We have mentioned just a few uses - you can probably suggest many more. Some of our customers are presently using this system for monitoring lab waste, reading wipe/smear tests, and uptake applications. Complete systems are available now! But, if you have some equipment and want to talk with our engineers about compatibility or discuss your particular requirements, just write or call, today. Let us send you free brochures describing these and other fine nuclear instruments for quality assurance, health physics and teaching laboratories.

EXCELLENCE IN NUCLEAR INSTRUMENTATION

461 LABORATORY ROAD • OAK RIDGE, TN • 37830  
TELEPHONE 615-483-0008 • TLX 557-482

REPRESENTATIVES WORLDWIDE



# Now there's an economical agent


## AN-MDP™ Technetium Tc 99m Medronate Kit

If you've been waiting for an economical way to produce high-quality, low-background medronate (MDP) bone images, wait no more. AN-MDP™, from Ackerman Nuclear, Inc., gives you all of the advantages of medronate—and a lot of medronate for your money.

**Superior images**  
Medronate produces high-target-to-background scans that readily demonstrate altered osteogenesis.<sup>1</sup>

- 90-94% blood clearance by two hours after administration
- Lowest soft-tissue uptake of all of the phosphonate bone agents in current use.<sup>2</sup>

- Convenience**
- When necessary, imaging may begin an hour after injection (optimal imaging time is 1 to 4 hours).
  - AN-MDP is stored and used at room temperature (15-30°C).
- Economy**
- You get 6 vials of reagent with each AN-MDP kit, instead of the usual 5.

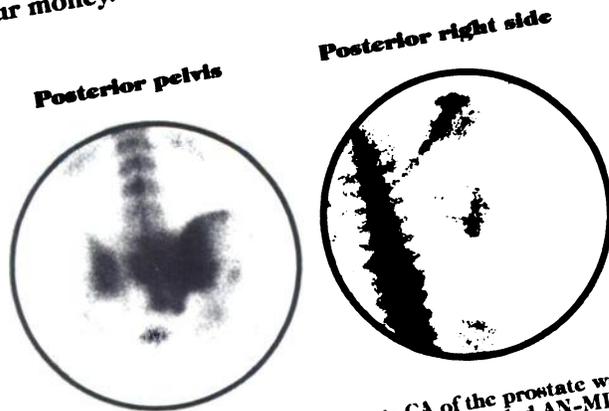

A 54-year-old male with metastatic CA of the prostate was administered 15 mCi technetium Tc 99m-labeled AN-MDP. The images were recorded at 500K counts. Courtesy of Century City Hospital, Los Angeles.

For complete prescribing information, consult the package insert, a summary of which follows.

### AN-MDP™ Technetium Tc 99m Medronate Kit

**Indications and usage.** Technetium Tc 99m Medronate may be used as a bone imaging agent to delineate areas of altered osteogenesis.

**Contraindications.** None known.

**Warnings.** This class of compounds is known to complex calcium. Particular caution should be used with patients who have or who may be predisposed to hypocalcemia (i.e., alkalosis).

**Precautions.** Contents of the vial are intended only for use

in the preparation of Technetium Tc 99m Medronate and are NOT to be administered directly to the patient. Technetium Tc 99m Medronate, as well as other radioactive drugs, must be handled with care and appropriate safety measures should be used to minimize radiation exposure to patients consistent with proper patient management.

To minimize radiation dose to the bladder, patients should be encouraged to drink fluids and to void immediately before the examination and as often thereafter as possible for the next 4-6 hours.

Technetium Tc 99m Medronate should be formulated within six (6) hours prior to clinical use. Optimal imaging results are obtained 1-4 hours after administration.

Carcinogenesis, mutagenesis, impairment of fertility. No long-term animal studies have been performed to evaluate

carcinogenic potential or whether Technetium Tc 99m Medronate affects fertility in males or females.

**Pregnancy category C.** Animal reproductive studies have not been conducted with Technetium Tc 99m Medronate. It is also not known whether Technetium Tc 99m Medronate can cause fetal harm when administered to a pregnant woman or can affect reproduction capacity. Technetium Tc 99m should be given to a pregnant woman only if clearly needed. Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

**Nursing mothers.** Technetium Tc 99m is excreted in human milk during lactation, therefore formula feedings should be substituted for breast feedings.

# for those famous "MDP" scans.

- **CUT WASTE.** You can choose either single-dose or multi-dose vials to match your department's volume.
  - For greater savings, both single-dose and multidose AN-MDP come in 30-vial ECONO-PAKS.
- Join the hundreds of nuclear medicine departments who


already enjoy the benefits of "MDP" scans. To place your order today, just call us collect: (213) 240-8555.

1. Davis MA, and Jones AG: *Sem Nucl Med* 6:19, 1976
2. Subramanian G, McAfee JG, Blair RJ, Kalfelz FA, and Thomas FD: *J Nucl Med* 16:744, 1975

Ackerman Nuclear, Inc.  
445 West Garfield Avenue  
Glendale, CA 91204  
(213) 240-8555



ACKERMAN NUCLEAR, INC.

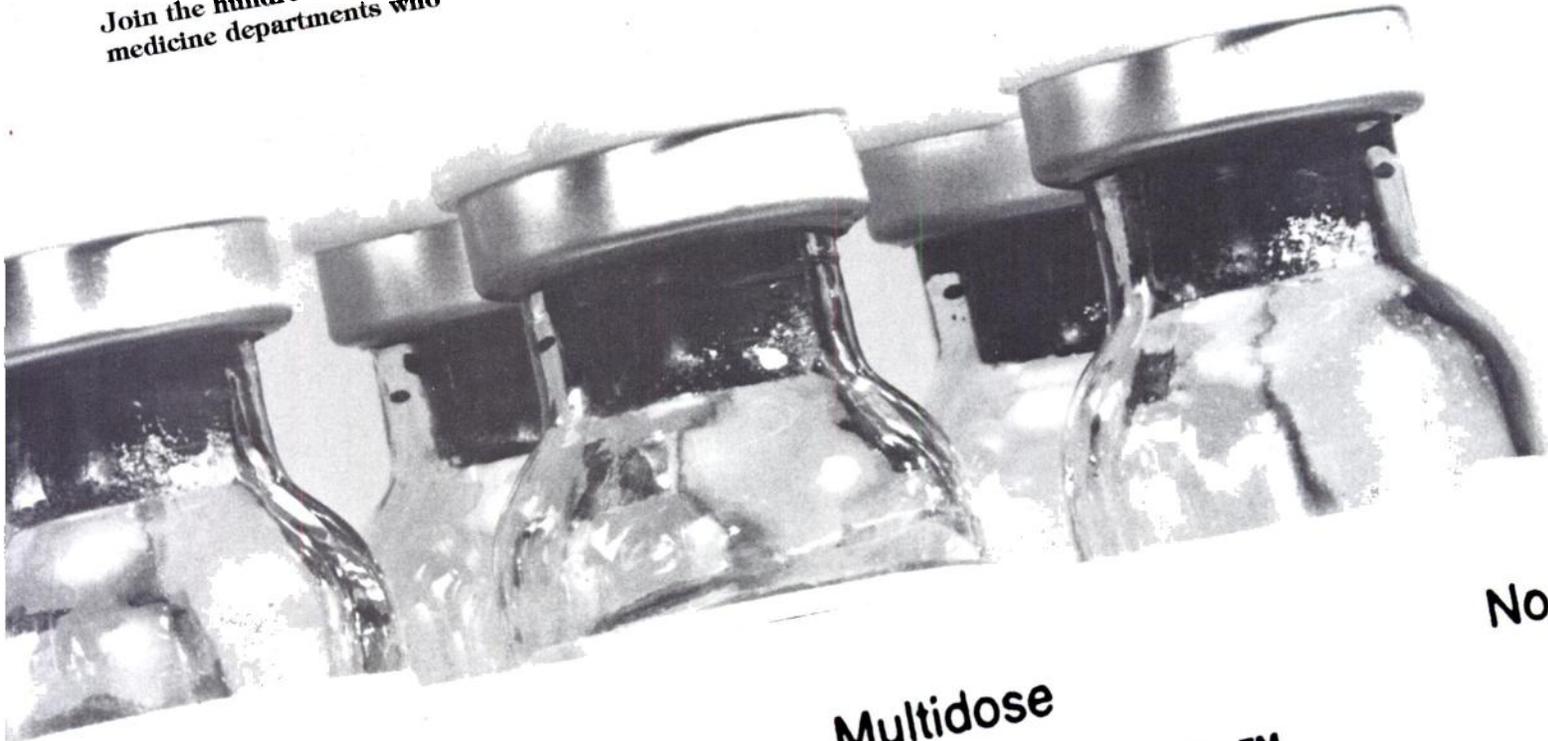

sterile

Multidose

# AN - MDP™

# MEDRONATE

Non

Pediatric use. Safety and effectiveness in children have not been established.

Radiopharmaceuticals should be used only by physicians who are qualified by training and experience in the safe use and handling of radionuclides and whose experience and training have been approved by the appropriate government agency authorized to license the use of radionuclides.

**Adverse reactions.** No adverse reactions specifically attributable to the use of Technetium Tc 99m Medronate have been reported.

**Dosage and administration.** The suggested dose range for i.v. administration after reconstitution with oxidant-free sodium pertechnetate Tc 99m injection to be employed in the average patient (70 kg) is

Bone imaging: 10-20 mCi Technetium Tc 99m Medronate

Scanning is optimal at about 1-4 hours post-injection. The patient dose should be measured by a suitable radioactivity calibration system immediately prior to administration.

**How supplied.** AN-MDP™ is supplied both in the single-dose and multidose form. Both are available in sets of 6 or 30 sterile and nonpyrogenic vials. Each nitrogen-flushed vial contains, in lyophilized form

	Single dose	Multidose
Medronic acid	5.0 mg	10.0 mg
Stannous chloride (minimum)	0.25 mg	0.51 mg
Maximum total stannous and stannic chloride	0.51 mg	1.01 mg

The pH is adjusted to 5.0-5.5 with HCl and NaOH prior to lyophilization. Included in each 6-vial kit is one package insert and 12 radiation labels. In each 30-vial kit is one package insert and 60 radiation labels. Refrigeration is not necessary.

Description	Catalog Number
Single dose 6-vial kit	K-401-S
Single dose 30-vial ECONO-PAK	K-402-S
Multidose 6-vial kit	K-401
Multidose 30-vial ECONO-PAK	K-402

AN-MDP™ is a trademark of Ackerman Nuclear, Inc.

# NEW THE XenaCon FROM RADX



A spirometer xenon rebreathing device for less than \$2500!!! Impossible? Almost, but we did it! We used the technology and know-how gained from 5 years of experience with the Ventil-Con and created the first low-cost spirometer xenon unit.

**XenaCon I** basic spirometer unit

**XenaCon II** spirometer unit with built-in Xenon Trap

**XenaCon III** spirometer unit with Xenon Trap and Xenon Trap Exhaust Port Monitor detector/alarm system

## PERTINENT SPECIFICATIONS

**Mobility:** all units are highly mobile, making bedside studies practical

**Unit dead space:** less than 25 ml in both washout and rebreathing

**Spirometer volume:** 0-10 liters

**Breathing resistance:** less than 0.1 inch of water to normal breathing

**Shielding:** spirometer area — 1/8 inch lead trap area — 1/4 inch lead

**Oxygen replenishment:** manual pushbutton valve

**Xenon injection port:** located in head valve for either direct bolus or homogeneous mixture patient administration

**Bacteriological filter:** inline autoclavable bacteriological filter

**CO<sub>2</sub> trap:** high capacity, easy access CO<sub>2</sub> trap

**Xenon trap cartridge pack:** New vertical activated Charcoal cartridge pack eliminates channeling

For more information, call or write Radx today.

## **RADX**

P.O. Box 19164 • Houston, Texas 77024

713-468-9628



...OR

# SEND YOUR SURVEY METERS TO THE EXPERIENCED PROFESSIONALS FOR CALIBRATION.

**Health Physics Associates, Ltd.**, servicing the radiation safety field since 1961, specializes in survey meter repair and calibration...with guaranteed results. All work is performed Accurately, Promptly and Thoroughly by electronic specialists and supervised by qualified physicists certified by the American Board of Health Physics. Instrument calibration is normally **completed in 24-48 hours**. Health Physics Associates, Ltd., services most radiation safety instruments including Geiger Counters, Ionization Chambers, Portable Scintillation Counters, and Direct and Indirect Reading Dosimeters. These services include:

- full preventive maintenance check
- repair and replace all defective components
- all services fully insured
- zero drift and radiation field drift checks
- calibration accuracy of  $\pm 10\%$
- meets or exceeds all Federal, State, Local and JCAH requirements
- shipping cases and loaner instruments available

**INSTRUMENT SERVICE RECORD**

Model # \_\_\_\_\_ Serial # \_\_\_\_\_

Calibration Date \_\_\_\_\_

Calibration Source \_\_\_\_\_

Maintenance Date \_\_\_\_\_

Due for Recalibration \_\_\_\_\_

This instrument meets NRC 10 CFR 34.24 standards. It should be returned for recalibration on date shown for compliance with above and various states requirements. Return to:

**HEALTH PHYSICS ASSOCIATES, LTD.**

**Health Physics Associates, Ltd.**, also offers these services:

- Leak/wipe tests (mail or personal)
- NRC and State License preparation
- Radiation safety services to meet NRC and State regulations (e.g. Surveys, calibrations, standards)
- Quality Assurance Programs for Nuclear Medicine Departments
- Continuing education programs for staff and laboratory personnel
- Decontamination services
- Emergency room radioactivity services

For more information, write or call us.

**HEALTH PHYSICS ASSOCIATES, LTD.**


3304 Commercial Avenue  
Northbrook, IL 60062  
312/564-3330

*Providing Radiation Safety Services Since 1961*

**Please send more information on:**

NAME	TITLE
HOSPITAL	DEPARTMENT
ADDRESS	
CITY	STATE
	ZIP CODE

# A dynamic quantitative study of rCBF

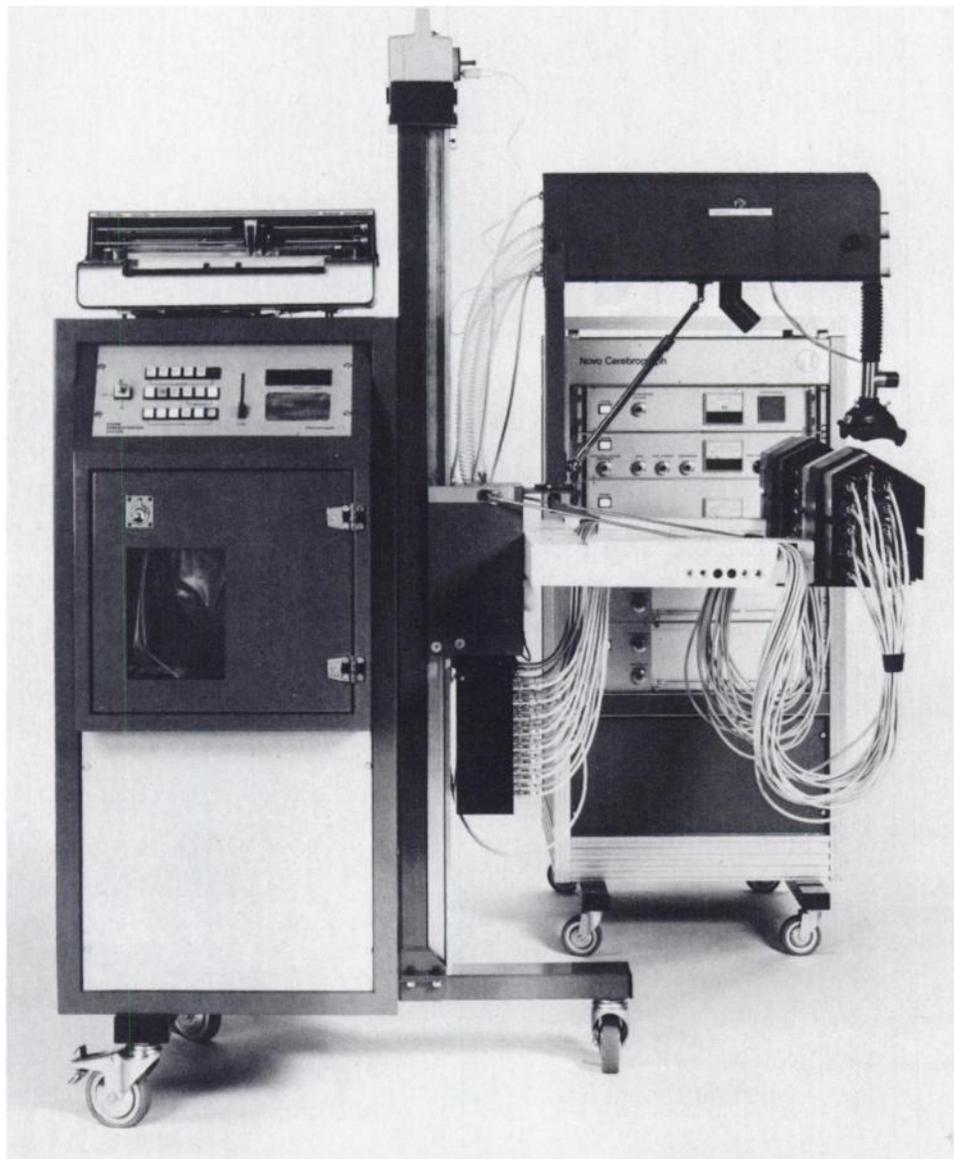

**The Novo Cerebrograph gives you dynamic quantitative measurement of regional Cerebral Blood Flow.**

Computerized digital and graphical printouts provide on-the-spot data on the functional level of the brain, data that cannot be obtained by other investigative methods.

And the *Novo Cerebrograph* gives you a choice of three  $^{133}\text{Xenon}$  administration techniques: inhalation, intravenous or intracarotid injection.

Using the  $^{133}\text{Xenon}$  inhalation method or the intravenous method, a safe and simple measurement of rCBF is obtained. It eliminates the trauma of intracarotid artery puncture. Permits simultaneous bilateral measurements, enabling an unaffected hemisphere to serve as reference for an affected one. Is widely used for research volunteers and on a broad patient spectrum for frequent measurements over prolonged periods.

The  $^{133}\text{Xenon}$  intracarotid injection method provides higher resolution, increases accuracy on white matter flow measurements, and is normally combined with a carotid angiogram.

When you buy a *Novo Cerebrograph* you get a complete system, including a pushbutton Xenon administration system with trap. Optional Xenon Recovery Unit. An air-detector. Up to 32 brain detectors with interchangeable collimators. A mobile detector stand that permits measurements with patients sitting or supine. Nuclear electronics and accumulation interface rack-mounted in cabinet. And your choice of on-line table-top or off-line data calculators and clinically verified proprietary computer programs.

## NOVO DIAGNOSTIC SYSTEMS A/S

(formerly Meditronic A/S)

Novo Allé  
DK-2880 Bagsvaerd (Denmark)  
Phone: (02)982333  
Telex: 27116  
Cable: Telanovo

46A

THE JOURNAL OF NUCLEAR MEDICINE

B 217-1979

OSTEOLITE bone imaging in oncology

The superior  
technique:

“Perhaps the greatest contribution of bone imaging is its superiority over conventional radiography in the detection of metastatic bone tumors.”<sup>1</sup>

1. J Nucl Med 19:324, 1978



The superior  
agent:

**OSTEOLITE**<sup>TM</sup>

Technetium Tc 99m Medronate Sodium Kit (MDP)

**NEN** New England Nuclear®

# In oncology. for reliable early detection of bone metastases:

## Most rapid blood clearance<sup>2</sup>

- At 90 minutes postinjection, blood clearance of MDP pharmacologically identical to OSTEOLITE was approximately equal to that of tested pyrophosphate agents at 6 hours postinjection.
- At 3 hours, MDP blood levels were considerably less than those of tested EHDP and pyrophosphate.

**Result: low-background studies, whether you must scan early to meet patient-flow demands, or at 3 hours for more optimal image detail.**

## Lowest soft tissue activity<sup>2,3</sup>

The "difference in soft tissue activity (highest with polyphosphate and lowest with MDP) is discernible in clinical images."<sup>2</sup> A University of Minnesota study found that only 4% of 175 MDP images showed moderate to marked soft tissue activity, compared to 17% of EHDP images.<sup>3</sup>

**Result: highest assurance of visualizing all skeletal structures.**

## Highest target-to-background differential<sup>4</sup>

OSTEOLITE's rapid blood clearance and lower soft tissue uptake usually enable current gamma cameras to resolve peripheral skeletal structures and phalanges.

**Result: confidence of detecting resolution-challenging alterations in osteogenesis...even roentgenographically "invisible" fractures and small metastases.**

## Convenient storage and preparation

Available in 5-vial or 30-vial "Convenience Packs," OSTEOLITE can be stored and used at room temperature (15–30 C).

#### REFERENCES:

1. Harcke HT Jr. *J Nucl Med* 19:324, 1978
2. Subramanian G et al. *J Nucl Med* 16:744, 1975
3. Forstrom L et al: Data on file at New England Nuclear, Medical Diagnostics Division, North Billerica, MA
4. Davis MA, Jones AG. *Sem Nucl Med* 6:19, 1976

# OSTEOLITE™

Technetium Tc 99m Medronate Sodium Kit (MDP)



L Lat



R Lat



Base view

Images produced with 20.5 mCi technetium-99m labeled OSTEOLITE; spot images recorded at 500 K counts, Searle LFOV™ camera with Micro Dot™ Imager.

A 19-year-old male with known eosinophilic granuloma involving the mandible bilaterally was referred for a bone scan to rule out occult sites of involvement. Bone imaging with OSTEOLITE showed increased uptake in the rami of the mandible on both sides. The medial portion of the mandible anteriorly and the remainder of the skull, the spine, ribs, pelvis and long bones show no abnormalities suggestive of multiple foci of disease. The increased area of uptake around the left ankle was attributed to soft tissue swelling due to a recent ankle sprain.

Please see following page for full prescribing information.

**NEN** New England Nuclear®

# OSTEOLITE™

## Technetium Tc 99m Medronate Sodium Kit (Formerly Known as MDP)

October 1977

**DESCRIPTION:** New England Nuclear's OSTEOLITE™ Technetium Tc 99m Medronate Sodium Kit (formerly known as MDP), is supplied sterile and non-pyrogenic in lyophilized kit form suitable for reconstitution with sodium pertechnetate Tc 99m to form a diagnostic skeletal imaging agent for intravenous administration. Each vial contains 10mg medronate disodium, and 0.85mg stannous chloride dihydrate; pH is adjusted to between 7.0–7.5 with hydrochloric acid and/or sodium hydroxide solution. The contents of the vial are lyophilized and stored under nitrogen.

### PHYSICAL CHARACTERISTICS

Technetium Tc 99m decays by isomeric transition with a physical half-life of 6.02 hours. (SOURCE: Martin, M. J. Nuclear Data Project, Oak Ridge National Laboratory, March, 1976.) Photos that are useful for imaging studies are listed in Table 1.

**Table 1. Principal Radiation Emission Data—Technetium Tc 99m**

Radiation	Mean %/Disintegration	Mean Energy (keV)
Gamma-2	88.96	140.5

To facilitate correction for physical decay of Technetium Tc 99m, the fractions of initial activity that remain at selected intervals after the time of calibration are shown in Table 2.

**Table 2. Physical Decay Chart: Technetium Tc 99m Half-Life 6.02 Hours**

Hours	Fraction Remaining	Hours	Fraction Remaining
0 <sup>c</sup>	1.000	8	.398
1	.891	9	.355
2	.794	10	.316
3	.708	11	.282
4	.631	12	.251
5	.562	18	.126
6	.501	24	.063
7	.447		

<sup>c</sup>Calibration Time

### EXTERNAL RADIATION

The specific gamma ray constant for Technetium Tc 99m is 0.8R/mCi-hr. at 1cm. The half value layer is 0.2mm of Pb. To facilitate control of radiation exposure from millicurie amounts of Technetium Tc 99m, the use of a 6.35mm thick standard radiation elution lead shield will attenuate the radiation emitted by a factor greater than 10<sup>4</sup>.

**Table 3. Radiation Attenuation By Lead Shielding**

Shield Thickness (Pb)mm	Coefficient of Attenuation
0.2	0.5
0.95	10 <sup>-1</sup>
1.8	10 <sup>-2</sup>
2.7	10 <sup>-3</sup>
3.6	10 <sup>-4</sup>
4.5	10 <sup>-5</sup>
5.4	10 <sup>-6</sup>
6.3	10 <sup>-7</sup>

**CLINICAL PHARMACOLOGY:** Upon intravenous injection, Technetium Tc 99m OSTEOLITE exhibits a specific affinity for areas of altered osteogenesis. In humans, blood levels fall to 4-10% of the injected dose by two hours post-injection and to 3-5% by three hours. During the first 24 hours following its administration in patients with normal renal function, 50-75% of the radioactivity is excreted into the urine and less than 2% of the injected dose remains in the vascular system.

Uptake of the Technetium Tc 99m in bone appears to be related to osteogenic activity and to skeletal blood perfusion. The deposition in the skeleton is bilaterally symmetrical, with increased accumulation in the axial structure as compared to the appendicular skeleton. There is increased activity in the distal aspect of long bones as compared to the diaphyses. In pediatric patients, in whom the epiphyseal centers are still open, there is more marked accumulation of the radiopharmaceutical in the distal aspects of long bones than is seen in adults in whom the epiphyseal centers are closed. Localized areas of abnormal accumulation of the radiopharmaceutical may be seen in primary skeletal malignancies, metastatic malignancies to bone, acute or chronic osteomyelitis, arthritides, recent fractures, areas of ectopic calcification, Paget's disease, regional migratory osteoporosis, areas of aseptic necrosis and, in general, any pathological situation involving bone in which there is increased osteogenic activity or localized increased osseous blood perfusion. Since increased osteogenic activity and localized increased osseous blood perfusion are not usually present in chronic bone diseases, bone imaging agents, in general, are not effective in detecting such diseases. Localized areas of decreased accumulation of the radiopharmaceutical may be noted in areas of bone which have received localized fields of external radiation or to which blood flow has been interrupted. OSTEOLITE has also been noted to accumulate in areas of acute myocardial infarction from one to fourteen days after the pathologic event.

**INDICATIONS AND USAGE:** Technetium Tc 99m OSTEOLITE may be used as a bone imaging agent to delineate areas of altered osteogenesis.

**CONTRAINDICATIONS:** None known.

**WARNINGS:** The contents of the OSTEOLITE vial are intended only for use in the preparation of Technetium Tc 99m medronate sodium and are NOT to be directly administered to the patient.

Ideally, examinations using radiopharmaceuticals—especially those elective in nature—of women of childbearing capability should be performed during the first ten days following the onset of menses.

**PRECAUTIONS:** A thorough knowledge of the normal distribution of intravenously administered Technetium Tc 99m medronate sodium is essential in order to accurately interpret pathologic studies.

Technetium Tc 99m medronate sodium, as well as any radioactive agent, must be handled with care. Once sodium pertechnetate Tc 99m is added to the kit, appropriate safety measures should be used to minimize external radiation exposure to clinical personnel. Care should also be taken to minimize radiation exposure to patients in a manner consistent with proper patient management.

The Technetium Tc 99m labeling reaction involved in preparing Technetium Tc 99m medronate sodium depends on the maintenance of tin in the divalent state. Any oxidant present in the sodium pertechnetate Tc 99m employed may adversely affect the quality of the prepared agent. Thus, sodium pertechnetate Tc 99m containing oxidants should not be used without first demonstrating that it is without adverse effect on the properties of the resulting agent.

The use of bacteriostatic sodium chloride as a diluent for sodium pertechnetate Tc 99m may adversely affect the biologic distribution of the prepared agent, and its use is not recommended.

Adequate reproduction studies have not been performed in animals to determine whether this drug affects fertility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Technetium Tc 99m medronate

sodium should be used in pregnant women only when clearly needed.

It is not known whether this drug is excreted in human milk. As a general rule nursing should not be undertaken when a patient is administered radioactive material.

Safety and effectiveness in children have not been established.

**ADVERSE REACTIONS:** None reported.

**DOSAGE AND ADMINISTRATION:** The recommended dose for the average 70kg adult patient is 15mCi with a range of 10-20mCi. The patient dose should be measured by a suitable radioactivity calibration system immediately prior to administration.

Optimal imaging results are obtained within one to four hours after administration.

OSTEOLITE should be used within six hours after aseptic reconstitution with sodium pertechnetate Tc 99m. For optimum results this time should be minimized.

The vial contains no bacteriostat.

Radiopharmaceuticals should be used by persons who are qualified by specific training in the safe use and handling of radionuclides produced by nuclear reactor or particle accelerator and whose experience and training have been approved by the appropriate governmental agencies authorized to license the use of radionuclides.

### RADIATION DOSIMETRY

The estimated absorbed radiation dose to an average patient (70kg) from an intravenous injection of a maximum dose of 20 millicuries of Technetium Tc 99m OSTEOLITE is shown in Table 4.

**Table 4. Absorbed Radiation Dose**

Organ	Technetium Tc 99m Medronate Sodium (rads/20mCi)
Total Body	0.13
Bone Total	0.70
Red Marrow	0.56
Kidneys	0.62
Liver	0.16
Bladder Wall	2 hr void 2.60 4.8 hr void 6.20
Ovaries	2 hr void 0.24 4.8 hr void 0.34
Testes	2 hr void 0.16 4.8 hr void 0.22

Method of calculation: A Schema for Absorbed-Dose Calculations For Biologically Distributed Radionuclides, Supplement No. 1, MIRD Pamphlet No. 1, p. 7, 1968.

**HOW SUPPLIED:** NEN's OSTEOLITE™ Technetium Tc 99m Medronate Sodium Kit is supplied as a set of five or thirty vials, sterile and non-pyrogenic. Each nitrogen-flushed vial contains in lyophilized form:

Medronate Disodium—10mg  
Stannous Chloride Dihydrate—0.85mg

The pH is adjusted to between 7.0–7.5 with hydrochloric acid and/or sodium hydroxide solution. The contents of the vial were lyophilized under nitrogen. Store at room temperature (15°-30° C). Included in each five (5) vial kit is one (1) package insert and six (6) radiation labels. Included in each thirty (30) vial kit is one (1) package insert and thirty-six (36) radiation labels.

**INSTRUCTIONS FOR PREPARATION OF TECHNETIUM Tc 99m OSTEOLITE:** Aseptically inject 2 to 8ml of sodium pertechnetate Tc 99m (pertechnetate in isotonic saline without a bacteriostat) into the supplied vial of OSTEOLITE enclosed by a radiation shield. Swirl for at least ten seconds to dissolve completely. Label appropriately. Suitable labels have been supplied with each OSTEOLITE Kit. Use within six hours after reconstitution. For optimum results, this time should be minimized.

Using proper shielding, the vial containing the reconstituted solution should be visually inspected to insure that it is clear and free of particulate matter.

The contents of the kit vials are not radioactive; however, after reconstitution with sodium pertechnetate Tc 99m the contents are radioactive and adequate shielding and handling precautions must be maintained.

Do not use if there is a vacuum in the immediate drug container or if air is injected into the container when the dose is withdrawn.

Catalog Number NRP-420 (5 vial kit)  
Catalog Number NRP-420C (30 vial kit)



**New England Nuclear**  
**Medical Diagnostics Division**

601 Treble Cove Rd., North Billerica, MA 01862  
Call toll-free: 800-225-1572 Telex: 94-0996  
(In Massachusetts and International: 617-482-9595)

Canada: NEN Canada, 2453 46th Avenue, Lachine, Que. H8T 3C9  
Tel: 514-636-4971

Europe: NEN Chemicals GmbH, D-6072 Dreieich, W. Germany,  
Postfach 401240 Tel: (06103) 85034 Order Entry: (06103) 81013

# If you're getting all these advantages from your TSH RIA Kit, you must be using ours



## Quick reliable results

Tests are completed in one working day — with excellent reproducibility within and between batches.

## Room Temperature Incubation

Eliminates the use of a water bath for the incubation stages.

## Colour coding reduces missed tubes

And indicates adequate mixing of reagents.

## New TSH RIA Kit

Examine the advantages of our new kit for yourself, and discover the optimum balance we have achieved in assay performance, reliability and service.




The  
Radiochemical  
Centre  
Amersham

# WHEN YOU DO SOMETHING YOU GET TO BE VERY



November 8, 1895, fifteen years after the founding of Eastman Kodak Company, Wilhelm Roentgen discovered a "new kind of light" that he called x-rays, and quickly made the first radiograph of a human subject—his wife's hand.

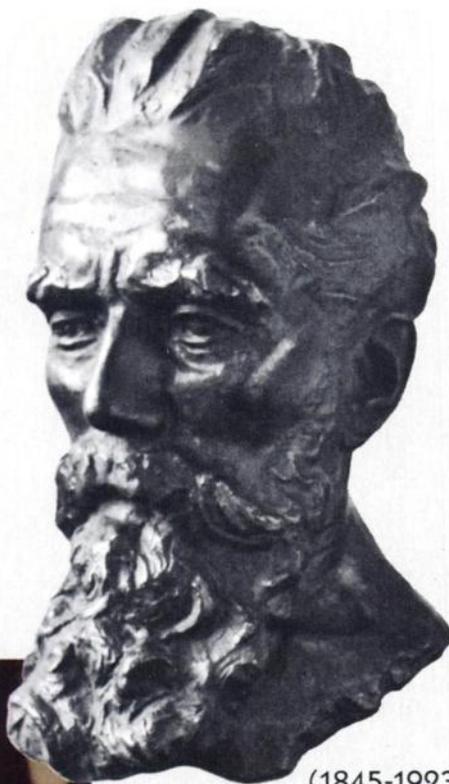

(1845-1923)  
Wilhelm Konrad Roentgen



Physicians discovered photography early, and used photos for teaching and record keeping. They were among Kodak's first customers.

An early Kodak darkroom lamp was a candle in a red fabric box. Today's Kodak safelight filter type GBX is "universal" and safe with all blue- and most green-sensitive x-ray films.



The first Kodak "demonstrator" was hired in 1884. Today, Kodak technical sales representatives call on the medical profession to provide imaging expertise and backup.



# FOR A VERY LONG TIME... GOOD AT IT.



Imaging is not complete without proper processing. An early Kodak advertisement showed a Kodak film processor that operated by turning a crank. The new Kodak RP X-Omat processor, model M8, processes x-ray film in 90 seconds and monitors its own performance automatically.




Nuclear medicine



Computed tomography



Ultrasound




CRT color photography

Kodak Lanex screens and Kodak ortho films provide quality images with reduced exposure and increased technic flexibility.



New imaging modalities require new products. If there is an image to be recorded, there is a Kodak film on which to record it.

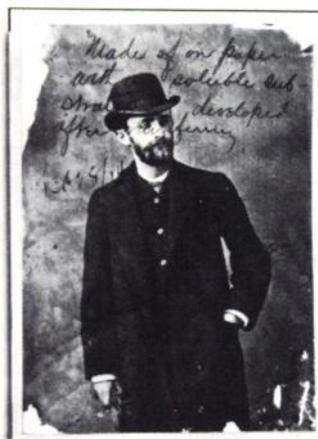

George Eastman, 1854-1932. He started it all.

1880



1980

100 YEARS OF TURNING  
ENERGY INTO IMAGES

# MEMO

## Nuclear Medicine

TO: PURCHASING

RE: THE C.I.S. REP WAS

By. THEIR IMAGING KITS

ARE WHAT WE PREFER.

CONVENIENT, CONSISTENT, RELIABLE

AND ECONOMICAL

THEIR FREE SAMPLE PERFORMED WELL

FOR OUR NEXT ORDER

CALL CIS AT

800-225-1145



**CIS Radiopharmaceuticals, Inc.**

5 DeAngelo Drive / Bedford, MA 01730 / Tel:(617) 275-7120  
Outside Massachusetts (800) 225-1145 / Telex 94-9465

When Toshiba gave nuclear medicine the world's first jumbo gamma-camera in 1973, the medical community was very impressed. But we were dedicated to giving you more, so we introduced the world's first jumbo gammacamera with high resolution, fine diagnostic detail over a large area. That was important, but we knew it still wasn't enough.

Now, we are introducing the latest in the state-of-the-art, the GCA-402. The world's first Super High Resolution, Large Field Gammacamera combining stability and exceptional workload capability in one instrument. Frankly, we're pleased.

Toshiba's system approach allows for no compromise where clinical diagnostic values are concerned. The GCA-402 is a prime example. High resolution is the basis for obtaining useful diagnostic images. The intrinsic resolution and linearity of the GCA-402, combined with its range of ten collimators provides unsurpassed images of exceptional diagnostic value. The GCA-402 incorporates 61 photo-multiplier tubes to electronically smooth the image and eliminate the high-energy collimator hole patterns unavoidable in conventional systems. Its 35cm field of view combined with 17 preselected isotope ranges allows unobstructed views of large organs, or groups of organs, as well as whole body scanning.

Toshiba's patented\* delay line system and modern IC-technology provide long term stability, trouble free performance, and ease of operation.

Of course, the GCA-402 has a wide range of accessories including special collimators, whole body scanning bed, video tape and film recorders, plus, the GCA-402 may be interfaced to any computer.

This combination of human engineering, fail-proof auto exposure and easy collimator changeover provides the highest efficiency while minimizing patient discomfort.

When you're ready to fill your nuclear medicine department's need for a large field gammacamera, remember Toshiba. We're the first.

\*Patented Delay Line, U.S. Patent Number 3,717,763

# Our third is first again

Toshiba's GCA-402 Jumbo Gammacamera



**TOSHIBA**  
MEDICAL SYSTEMS  
In Touch with Tomorrow

Division Of Toshiba International Corporation  
1154 Dominguez St., Carson, California 90745 (213) 638-5153

# ADAC. It has a

Some nuclear medicine computers are here today and obsolete tomorrow.

Not ADAC.



Take the very first system we ever made (Serial No. 76-001).

Today it can still *easily* handle every new clinical procedure developed for nuclear cardiology in the last five years.


This makes ADAC owners very happy.

Unlike non-ADAC owners. Who suffer the significant disadvantages of clinical obsolescence.


This is only one reason doctors have called the ADAC Nuclear Medicine Computer the finest system of its kind in the world.

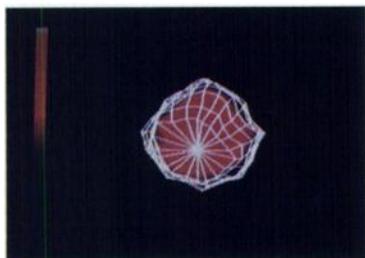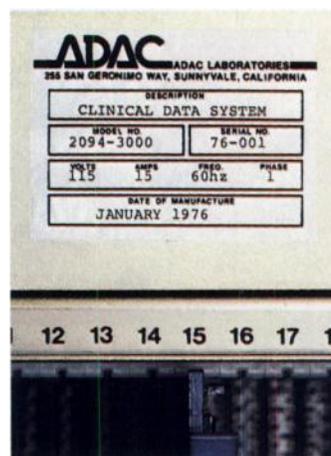


LAO

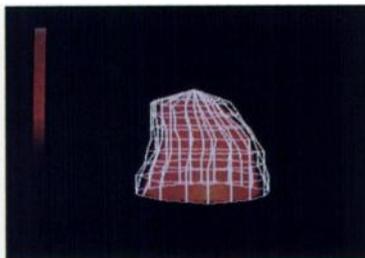

Inferior

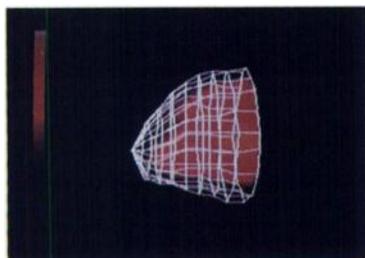

LPO

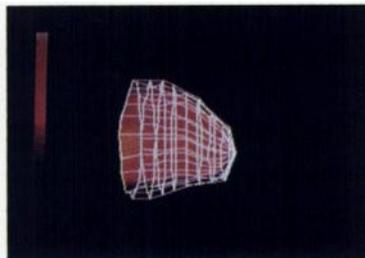

RAO

#### Shade Program:

A three dimensional representation of the left ventricle is constructed for each segment using the 8 areas of interest of each plane in each segment. The even spacing of the planes is known since it was specified to perform the reconstruction; therefore, the areas of interest, x and y dimensions, can be connected to create the depth, z dimension. The operator can specify the projection for the constructed three dimensional image or "birdcage." Rotation can be done on the heart's x, y and z axis. Clinically, it is very valuable to rotate to the RAO, LPO, Superior Aspect, and Inferior Aspect. For example, the RAO projection allows the viewing of the long axis of the left ventricle without the right ventricle superimposed, since the edge detection did not include the right ventricle.

# built-in future.

Why? Among other things, a  $512 \times 512$  display format and 64 shades of gray that deliver an image nearly identical to original analog scintiphotos.

And an easy-to-use computer language in plain English.

What's more, the cost is surprisingly low.

The message is clear. Make ADAC part of your future.

For additional information, please write or call collect.

ADAC Laboratories.

255 San Geronimo Way, Sunnyvale, California 94086. (408) 736-1101.

```
PATIENT DEMO READY FOR PROCESSING

PROCESSING OPTIONS:
1. USER DEFINED PROCESSING.
2. VIEW IDENTIFICATION.
3. RUN ANOTHER PROGRAM
4. BACKGROUND SUBTRACTION.
5. CONTRAST ENHANCEMENT.
6. FRAME ADDITION OR SUBTRACTION.
7. CHARACTER SUPERPOSITION.
8. DISPLAY IMAGES.
9. AREA OF INTEREST, PLOTTING, AND CURVE ANALYSIS.
10. TERMINATE THIS PROGRAM
8

DO YOU WANT TO DISPLAY:
1. SINGLE IMAGES.
2. MULTIPLE IMAGES SIMULTANEOUSLY.
3. MOTION PICTURES.
4. CYCLIC MOTION PICTURES.
5. RETURN TO PROCESSING OPTIONS.
```




## ADAC

Nuclear Medicine Computers

# THE STABLE SOLUTION TO YOUR BONE IMAGING NEEDS

NOW AVAILABLE FOR ROUTINE USE

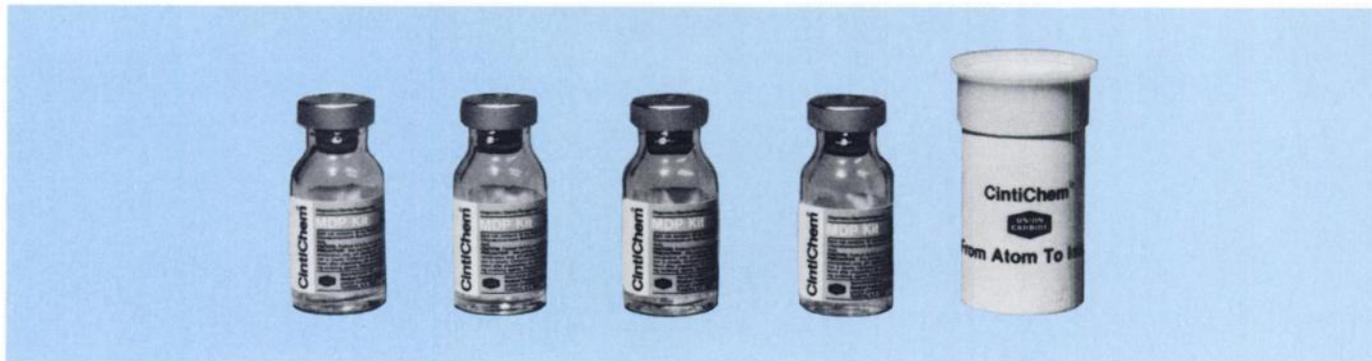

- One Year Shelf Life
- No Refrigeration Required
- Full 6 Hour Use After Preparation
- Contains Ascorbic Acid as an Antioxidant

For ordering, customer service, and technical information, call toll-free 800-431-1146 (in NYS call 914-351-2131, ext. 227).

**CintiChem<sup>®</sup>**  
**MDP<sup>KIT</sup>**

## Technetium Tc 99m Medronate Kit

### BRIEF SUMMARY OF PRESCRIBING INFORMATION

#### indications and usage

Technetium Tc 99m Medronate may be used as a bone imaging agent to delineate areas of altered osteogenesis.

#### contraindications

None known.

#### warnings

This class of compound is known to complex cations such as calcium. Particular caution should be used with patients who have, or who may be predisposed to, hypocalcemia (i.e., alkalosis).

This radiopharmaceutical drug product should not be administered to children, to pregnant women, or to nursing mothers, unless the expected benefit to be gained outweighs the potential risk.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

#### precautions

##### general

Technetium Tc 99m Medronate as well as other radioactive drugs, must be handled with care and appropriate safety measures should be used to minimize radiation exposure to clinical personnel. Also, care should be taken to minimize radiation exposure to the patients consistent with proper patient management.

To minimize radiation dose to the bladder, the patient should be encouraged to void when the examination is completed and as often thereafter as possible for the next 4-6 hours.

This preparation contains no bacteriostatic preservative. Technetium Tc 99m Medronate should be formulated within six (6) hours prior to clinical use.

##### pregnancy category C

Adequate reproductive studies have not been performed in animals to determine whether this drug affects fer-

tility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Technetium Tc 99m Medronate should be used in pregnant women only when clearly needed.

##### nursing mothers

It is not known whether this drug is excreted in human milk. As a general rule nursing should not be undertaken while a patient is on the drug since many drugs are excreted in human milk.

##### pediatric use

Safety and effectiveness in children have not been established.

#### adverse reactions

No adverse reactions specifically attributable to the use of Technetium Tc 99m Medronate have been reported.

#### how supplied

Union Carbide's Technetium Tc 99m Medronate Kit is supplied as a sterile, pyrogen-free kit containing 5 vials.

Each 10 ml vial contains 10 mg medronic acid, 0.17 mg (minimum) stannous chloride (maximum stannous and stannic chloride 0.29 mg), and 2 mg ascorbic acid. The pH has been adjusted to 4-8 with either HCl or NaOH prior to lyophilization. Following lyophilization, the vials are sealed under a nitrogen atmosphere.

Product #17500502 Multidose vial shield with cap and retainer ring available separately.



**FROM ATOM TO IMAGE**

Manufactured For:

Union Carbide Corporation • Medical Products Division •  
Nuclear Products • P.O. Box 324 • Tuxedo, New York 10987

CintiChem is a registered trademark of Union Carbide Corporation.

# LEAD ISN'T ALWAYS YOUR BEST PROTECTION... THE MEMORY AND REMOTE CHAMBER OF OUR CRC-30 ARE.



Our CRC-30 calibrator has a computer that helps reduce overall exposure. How? By computing the correct dose the first time. There are no "repeats", and the syringe is never "filled" or "emptied". Result: Less handling, less exposure. For both you, and the patient. To reduce operator exposure even further, we've designed our calibration chamber so that it can be physically isolated from the controls, a comforting feature.

**RADIOISOTOPE DOSE COMPUTATION AND MEASUREMENT RECORD**  
 PATIENT'S NAME: FRED BARNES  
 I.D. NO.: 087-61-3201  
 STUDIES: BRAIN SCAN  
 INCLUDE: TECHNETIUM 99m  
 FORM: PERTECH SAMPLE NO. 11  
 LOT NO.: 456-256  
 DATE: 29 AUG 75 12:23  
 CONCENTRATION: 00.01 mCi  
 DOSE DESIRED: 00.04 mCi  
 VOLUME REQUIRED: 000.6 uCi  
 ACTIVITY MEASD: 3.05  
 TIME OF ADMINISTRATION: 3:05  
 SIGNATURE: J. McKinley  
 CAPINTEC INC.

**RADIOCHEMICAL PURITY ANALYSIS AND DC CHROMATOGRAPHIC RECORD**  
 PHARMACEUTICAL: SULFUR COLLOID  
 PREP: WHATMAN #1  
 VIAL: NORMAL SALINE  
 TECHNETIUM 99m  
 -256uCi KIT NO. 24  
 VC 79 12:28

**PRE-CALIBRATION RECORD**  
 TECHNETIUM 99m  
 29 AUG 75

At Capintec, we are professionals. We take dose calibration and control very seriously. No wonder we're the world's best seller.

Capintec, Inc., 136 Summit Avenue, Montvale, NJ 07645.  
 (201) 391-3930. Toll Free  
 (800) 631-2557. TELEX 642375  
 CAPINTEC MTLE.

**CAPINTEC**  
 WE TAKE RADIATION SERIOUSLY.  
 THAT'S WHY SERIOUS BUYERS CHOOSE US.

## Baylor College of Medicine

TEXAS MEDICAL CENTER HOUSTON, TEXAS 77030



### NUCLEAR MEDICINE: MAJOR EXPAN— SION OF ESTABLISHED PROGRAM

#### OPPORTUNITIES FOR NM PHYSICIANS, MEDICAL SCIENTISTS, SUPERVISORY AND STAFF TECHNOLOGISTS, MEDICAL WRITER

A major expansion of an established program in NM is being developed in conjunction with the opening of a total health care center. The new program has created the need for qualified physicians, medical scientists and technologists to provide NM services for a 2500-bed hospital complex that includes 2 large cardiovascular centers.

Positions are immediately available for:

- (1) 3 NM physicians with clinical expertise in all aspects of nuclear medicine and interest in clinical research
- (2) 2 medical scientists with interest in instrumentation, computer science, and radiation physics
- (3) Several technologists, both staff and supervisory levels, for the imaging and RIA sections
- (4) Medical writer

For information contact John A. Burdine, M.D., Chief, Nuclear Medicine Section, Departments of Internal Medicine and Radiology, 6720 Bertner Avenue, Houston, TX 77030; phone 713/791-2272

### AMERICAN COLLEGE OF NUCLEAR PHYSICIANS

now offering

#### R.I.A. PROFICIENCY TESTING PROGRAM

**B5656-159A Survey I CORTISOL, DIGOXIN, FOLATE  
(100/yr) HGH, INSULIN, TBG, TSH, TRI-  
IODOTHYRONINE, T-4, B-12, T3  
UPTAKE**

**B5656-15SB Survey II same as Survey I + ESTRIOL, FSH,  
(\$180/yr) GASTRIN, ALDOSTERONE,  
DIGITOXIN, TESTOSTERONE,  
GENTAMYCIN, DILANTIN, HCG,  
FERRITIN**

SHIPPED QUARTERLY

Daily Quality Control Program Also Available.

For information call 202/857-1135 or write:

AMERICAN COLLEGE OF NUCLEAR PHYSICIANS  
Suite 700  
1101 Connecticut Avenue, N.W.  
Washington, D.C. 20036

THIS PROGRAM IS CONDUCTED IN COLLABORATION  
WITH DADE DIVISION, AMERICAN HOSPITAL SUPPLY  
CORPORATION

# WHEATON ZIPPETTES

## Better Than "The Best" For Less



New, improved Mark III Zippette dispensers are highly resistant to breakage. The borosilicate glass syringe is encased in protective polypropylene. Delivery valves are positioned within the reservoir for added safety. The delivery tip is secured by a rigid platform to eliminate dislodging by accident. Fully adjustable throughout syringe capacity. Five sizes available: 0-0.5 ml, 0-5 ml, 0-10 ml, 0-30 ml, 0-50 ml. Fully autoclavable without disassembly. Available with low profile, anti-tip, safety reservoir of amber glass, or one gallon amber plasti-coted bottle for the 0-30 ml and 0-50 ml sizes. Screw threaded adapters for use with common laboratory containers.

For complete information contact Wheaton Instruments.

 **WHEATON  
INSTRUMENTS**

1000 N. 10th Street, Millville, NJ 08332, U.S.A.

# PLACEMENT

## POSITIONS OPEN

**NUCLEAR MEDICINE TECHNOLOGIST.** A progressive, 419-bed hospital needs a Nuclear Medicine Technologist, who is registered or registry eligible. Individual will be working with Searle cameras, a mobile camera with computer, a whole body imager and a MDS computer. Excellent salary, working conditions, and fringe benefit program. Send resume or call: Personnel Office, Baptist Medical Center, P.O. Box 11010, Montgomery, AL 36111. (205) 288-2100, Equal Opportunity Employer.

**PATHOLOGY-NUCLEAR MEDICINE** Physician being sought to join practice in a 400 Bed community hospital. Send resume to William M. Bridger, M.D. Baptist Medical Center, 2105 East South Boulevard, Montgomery, Alabama 36116.

**NUCLEAR MEDICINE RESIDENCY.** Medical College of Wisconsin. Two year integrated program including 710 bed VA General Hospital, 600 bed County Medical Complex and two large community hospitals. Several cameras each interfaced to computer. Ultrasound training included. Positions available in July 1980. Nondiscrimination in employment. Contact Robert C. Meade, M.D., Chief, Nuclear Medicine Service, VA Center, Milwaukee, WI 53193. 414-384-2000, Ext 2138.

**NUCLEAR PHYSICIAN.** THE NEW YORK Hospital and Cornell University Medical College are seeking a Board certified or Board eligible Nuclear Physician with at least two years training in Nuclear Medicine. The successful candidate will fill a staff position in the Division of Nuclear Medicine at The New York Hospital and receive an academic appointment at Cornell University Medical College. Background in Radiology, Internal Medicine, or Pathology is acceptable. Candidates must be prepared to assume major clinical and teaching responsibilities; outstanding research opportunities also available. Appointment for July 1, 1980 or sooner. Contact David V. Becker, M.D., Chief, Division of Nuclear Medicine. The New York Hospital-Cornell Medical Center, 525 East 68th Street, New York, New York 10021.

**ASSISTANT CHIEF, NUCLEAR MEDICINE SERVICE.** The Minneapolis Veterans Administration Medical Center seeks candidate for the position of Assistant Chief, Nuclear Medicine Service effective July 1, 1980. Requirements include certification by the ABNM, a strong patient orientation and expertise in all phases of clinical nuclear medicine, including imaging, radioassay and internal radionuclide therapy. In addition, the Assistant Chief, Nuclear Medicine Service will have specific responsibilities in research and education. Applications from all qualified candidates are welcome. Inquiries, including a curriculum vitae and an autobiographical letter, should be sent to: Rex B. Shafer, M.D., Chief, Nuclear Medicine Service (115), Veterans Administration Medical Center, 54th Street & 48th Avenue South, Minneapolis, MN. 55417. An Equal Opportunity Employer.

**NUCLEAR MEDICINE (2 YR)/NUCLEAR Radiology (1 yr) residencies in combined University Hospital—VA Hospital program.** Training available in nuclear imaging and nuclear in vitro procedures. Opportunities for clinical and laboratory research. W. N. Tauxe, Director, Division of Nuclear Medicine, University of Alabama Hospitals, Birmingham, Alabama 35233.

**NUC. MED. TECH. SUPERVISOR-RIA & Wet Lab.** Immediate opening for an experienced supervisor in 1200 bed university hospital. Responsibilities include organizing, scheduling, and supervising the performance of all radioassay and wet lab procedures including evaluation of new tests. Prefer B.S. Degree in Medical Technology, Nuclear Medicine Technology, or Chemistry with several years of experience including supervisory duties. Registry or Certification in Nuclear Medicine Technology is required. Salary commensurate with experience plus full range of benefits. Casual living in semitropical climate. Send resume to William K. Otte, Jr., Technical Director, Nuclear Medicine, P.O. Box 146, University of Texas Medical Branch, Galveston, Texas 77550. UTMB is an EO Affirmative Action M/F/H Employer.

**UNIVERSITY OF PITTSBURGH** School of Medicine: Full-time position at the Asst./Assoc. Professor level; salary commensurate with experience; ABNM or ABR (NM competence) certification or eligibility required. Full range of imaging procedures; dedicated computer; cooperative clinical and research program with cardiology division. Contact Lewis W. Gumerman, Chief-Nuclear Medicine, Presbyterian-University Hospital, DeSoto at O'Hara Sts., Pittsburgh, PA 15213 (412) 647-3343.

**RADIOLOGIST, BOARD ELIGIBLE OR Certified:** to join three associates in the Department of Radiation Therapy and Nuclear Medicine. Complete therapy facilities, 18 MeV Varian, Theratron 780, Therasim Simulator, Superficial and Orthovoltage units. Fully equipped nuclear Medicine Department; three cameras, Adac computer, recti-linear scanner. Radiologist should have both radiation therapy and nuclear medicine training. 550 bed private hospital. Contact: John F. Mokrohisky, M.D., P.O. Box 2446, Green Bay, Wis. 54306. (414) 433-8184 or (414) 437-8517.

**NUCLEAR MEDICINE PHYSICIAN (ABNM).** Interested in clinical nuclear medicine Research & teaching in a university hospital environment. An academic appointment at the instructor, assistant or associate professor level is available depending upon credentials and experience. Contact Stanley J. Goldsmith, M.D., Director, Dept. of Physics-Nuclear Medicine. The Mount Sinai Medicine Center, One Gustave L. Levy Place, New York, NY 10029, (212) 650-7888. An equal opportunity employer.

**NUCLEAR MEDICINE TECHNOLOGIST.** Immediate opening for a Registered or Registry Eligible Nuclear Medicine Technologist with a private group of Pathologists. Responsibilities include both in vivo and in vitro studies with the latest equipment. Salary is negotiable. Apply or send resume to: Wabash County Hospital Clinical Laboratory/Nuclear Medicine 670 North East Street Wabash, Indiana 46992 (219-563-7132).

**NUCLEAR MEDICAL TECHNOLOGIST.** Immediate, excellent opportunity for an experienced registered or registry eligible Technologist. Will work in large department of a 700 bed General Hospital with forward looking ideas. The Department has 2 full-time Nuclear Physicians, a Physicist, 2 New GE Maxi-IIs, 2 Standard Cameras and computer. Associated with research facilities in Radioassay and Rheumatology. Position should provide an interesting opportunity with a busy but not boring atmosphere for a dedicated Technologist. Excellent employee benefits and opportunities. Submit credentials to Mr. Warren Garfield, Director of Personnel, Presbyterian Hospital of Dallas, 8200 Walnut Hill Lane, Dallas, Texas, 75231.

**EARL K. LONG MEMORIAL HOSPITAL** needs qualified Radioisotope Technologists who are registered or eligible for registry. A 250 bed teaching State Hospital with benefits of State employment. Straight day shift with some call time; I & II levels available. Contact: Frank West, Radiology, 5825 Airline Hwy., B.R., LA 70805. (504) 356-3316, ext. 216. An EEO Employer.

**NUCLEAR MEDICINE PHYSICIAN.** Applications are invited for a full-time position in the Department of Nuclear Medicine at University Hospital, Saskatoon, Saskatchewan. At present the staff consists of one full-time physician, one half-time physician, and a complement of two physicists. Services are provided to the population of the northern half of the province including two other hospitals in Saskatoon and the Saskatoon Clinic of the Saskatchewan Cancer Foundation. Teaching involves participation in undergraduate and postgraduate medical education and technology training programs. Opportunity exists for research. Applicants must hold or be eligible to sit the F.R.C.P. (C) examination in Nuclear Medicine. The successful applicant will be offered a teaching appointment at an appropriate academic rank in the Department of Diagnostic Radiology of the University of Saskatchewan. Please apply to: Dr. H. P. Kent, Head, Department of Diagnostic Radiology, University Hospital, Saskatoon, Saskatchewan, Canada S7N 0X0.

**NUCLEAR MEDICINE PHYSICIAN:** A physician who desires research experience in the Veterans Administration Nuclear Medicine Career Development Program (Research Associate or Clinical Investigator) contact Dr. Tapan Chaudhuri, VA Medical Center, Hampton, Virginia 23667, (804) 722-9961, Ext. 364, affiliated with Eastern Virginia Medical School.

**NUCLEAR MED TECH—ARE YOU** looking for a challenging position in the field of nuclear medicine? If you are registered or registry eligible and need a full time position, then this may be the opportunity you've been looking for. This is a beautiful university community with several lakes and parks in close proximity. Bloomington Hospital is a 314 bed Hospital that services Bloomington and the surrounding areas. If interested please call or write: Bloomington Hospital, 619 W. First St., Bloomington, In. 47401 (812) 336-9535. An Equal Opportunity Employer M/F.

**NUCLEAR MEDICINE TECHNOLOGIST or Registered X-Ray Technician,** with imaging experience, for Midwestern mobile medical scanning service. Position requires daily travel to area hospitals with mobile scanning equipment. Salary commensurate with experience. Excellent corporate fringe benefits. Position currently open in our Des Moines, Iowa, and Mankato, Minnesota, branch facilities. Send resume to Arlo Flanders, Personnel Director, Laboratory of Clinical Medicine, 1212 S. Euclid Avenue, Sioux Falls, S. Dak., 57105. Or call (800) 843-6811. Equal Opportunity Employer.

**NUCLEAR MEDICINE PHYSICIAN.** The Division of Nuclear Medicine at the Hospital of the Univ. of Pennsylvania has an opening at the Asst. Prof. level. Strong background in both clinical and research nuclear medicine desirable. Well equipped Division with modern imaging instruments, computers and a cardiovascular Nuclear Medicine facility in ICU area. PETT scanner will be installed shortly. Excellent research opportunities. Contact Abass Alavi, M.D., Chief, Division of Nuclear Medicine, Hospital of the University of Pennsylvania, 3400 Spruce Street, Philadelphia, PA 19104.

**MONTEFIORE HOSPITAL, UNIVERSITY of Pittsburgh School of Medicine** is seeking a full-time faculty member to direct the Nuclear Medicine Unit of the Department of Medicine. Applicants should have experience in advanced nuclear medicine and ultrasound techniques and be prepared to develop a program involving teaching, patient care and clinical research. Replies and curriculum vitae should be sent to: Philip Troen, M.D., Physician-in-Chief, Montefiore Hospital, Professor and Vice-Chairman, Department of Medicine, University of Pittsburgh School of Medicine, 3459 Fifth Avenue, Pittsburgh, PA 15213. University of Pittsburgh is an equal opportunity/affirmative action employer.

**UNIVERSITY OF MIAMI SCHOOL OF Medicine.** Full-time Academic position involving all aspects of Nuclear Imaging, Radioassay, Echocardiography and Doppler Ultrasound. Experience in Cardiovascular procedures preferred but not essential. Contact Aldo N. Serafini, M.D., Director, Division of Nuclear Medicine, University of Miami School of Medicine, P.O. Box 016960, Miami, Florida 33101.

**NUCLEAR MEDICINE RESIDENCY** available. July 1980. Two year accredited affiliated program including 700 bed VA General Hospital, 500 bed County Hospital and 1,000 bed Air Force Medical Center; an equal opportunity employer. Comprehensive training in basic sciences, laboratory sciences, computer technology, patient care services, and research. Contact Martin L. Nusynowitz, M.D., Division of Nuclear Medicine, University of Texas Health Science Center, San Antonio, Texas, 78284 (512) 691-7265.

**CONFIDENTIAL SERVICE NATION-**wide. We are a search firm dealing nationwide in the Health Care Industry. All fees paid by employer. Forward resume with salary requirements and location preferences to BMI, Health Care Division, P.O. Box 6457, Columbia, S.C. 29260, (803) 787-8710.

### POSITIONS WANTED


**RADIOLOGIST, ABR, UNIVERSITY** trained including fellowship nuclear medicine, seeks position. Reply Box 1200, Society of Nuclear Medicine 475 Park Ave., New York, N.Y., 10016.

**NUCLEAR MEDICINE PHYSICIAN-**37, ABNM desires associate professor level position at university affiliated hospital. Strong research and administrative background. Reply Box 1201, Society of Nuclear Medicine, 475 Park Ave. So., New York, NY 10016.

**ABNM CERTIFIED, QUALITY- AND** risk/benefit-conscious M.D.-Ph.D., with several years' teaching hospital experience and an interest in computer applications. Letters of reference immediately available from Harvard U. Reply Box 1202, Society of Nuclear Medicine, 475 Park Avenue So., New York, NY 10016.

**DESIRE PHYSICS/NUCLEAR MEDI-**cine Instructor position with a progressive hospital/community college. Presently chief technologist, ARRT, graduate AMA approved school, 4 yrs. clinical experience. Recent M.Ed. Degree, physics concentration, with 4 years of teaching experience. Prefer Upstate New York, mid-Atlantic States Area. Call, early evening, 717-645-5955.

**EXPERT ASSISTANCE BY EXPERI-**enced Nuclear Medicine Technologist. Available part time, Manhattan only, on fee for service basis. Ten years experience. In vitro and imaging techniques. Excellent references. Reply P.O. Box 1203, Society of Nuclear Medicine, 475 Park Avenue So., New York, New York, 10016.

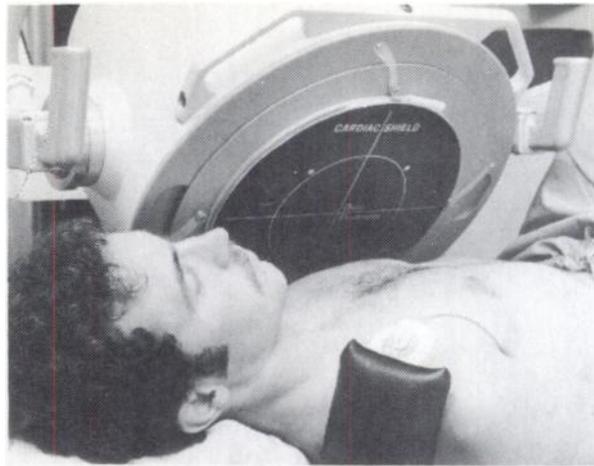

## CARDIAC SHIELD ELIMINATES NON-TARGET PHOTONS 7-day FREE trial!

\$95 SMALL, \$125 LARGE

Phone or write on your professional letterhead:  
**O'NEILL INC.**  
221 FELCH STREET,  
ANN ARBOR, MI, 48103  
AREA 313/973-2335



**BOARD CERTIFIED INTERNIST** completing University Residency in Nuclear Medicine July 1980. Age 48. Strong Computer background. Seeks position where he can be in charge and set his own hours, so that interest in Internal Medicine and Computers can be pursued secondarily. Reply Box 1204, Society Nuclear Medicine, 475 Park Ave., New York, NY 10016.

### FOR SALE

**BRATTLE PHYSIOLOGICAL SYN-**chronizer Model 202. New Condition. Contact Hans Tschersich, M.D., 1162 Willamette Street. Eugene, Oregon 97401. Phone (503) 687-6026.

**GAMMA CAMERA, SEARLE HP, 6** collimators, P Scope, Strip Chart Recorder, Good Detector. Best offer over \$10,000. Contact Ken Smith, 609-589-7859.

### STAFF NUCLEAR MEDICINE TECHNOLOGIST

Full time day shift position available for a Registered, Registry eligible or CNMT Nuclear Medicine Technologist. Rapidly expanding Nuclear Medicine department. Planned Nuclear Cardio Vascular Lab January 1980. Wadley Hospital is a modern 358-bed general acute care hospital. Good salary and employee benefits.

Please contact: Personnel Office (214) 794-7334

**Wadley Hospital**  
1000 Pine Street  
Texarkana, Texas 75501

# NUCLEAR MEDICINE TECHNOLOGIST

Nuclear Medicine Technologist to work in rapidly expanding 3 Tech. Nuclear Imaging Department in modern 600 bed JCAH advanced teaching hospital. No RIA. Computer experience helpful. Nuclear Medicine Registry or Registry eligible preferred. Please contact:



SAINT VINCENT

Mrs. Bea Gallo  
Professional Recruiter  
SAINT VINCENT  
HEALTH CENTERS  
P.O. Box 740  
Erie, PA 16544  
(814) 459-4000 Ext. 311

EQUAL OPPORTUNITY EMPLOYER

## UNIVERSITY OF CALIFORNIA SAN FRANCISCO SCHOOL OF MEDICINE

Nuclear Medicine resident positions are available beginning July 1, 1980 for a 2-year program at San Francisco General Hospital Medical Center.

The program, approved by the AMA and satisfying the requirements of the American Board of Nuclear Medicine, includes didactic instruction in radiologic physics and mathematics, electronics, radiation safety, dosimetry, and nuclear medicine instrumentation.

Practical experience is provided in performance and interpretation of static and dynamic imaging, computer techniques, radioimmunoassay and other in vitro tests, radiopharmacy, and therapy with radionuclides. Residents participate fully in the integration of these modalities into patient care.

Prerequisite: Prior training in AMA-approved program in pathology, radiology, internal medicine or pediatrics.

The University of California is an equal opportunity affirmative action employer.

Requests for further information (include CV) should be directed to:

Myron Pollycove, M.D.  
Chief, Nuclear Medicine  
San Francisco General Hospital  
Medical Center  
San Francisco, CA 94110

## BIOORGANIC CHEMIST

The Oak Ridge National Laboratory invites applications from highly qualified individuals with diversified training and interests. Experienced candidates with doctorate and postdoctoral training in synthetic organic chemistry, medicinal or pharmaceutical chemistry, biochemistry, radiopharmaceutical research or related areas will be considered. The duties involve the design, synthesis and preclinical testing of new radiopharmaceuticals for use in nuclear medicine. A new area will be the radiolabeling and testing of organic compounds that represent human health hazards. The position is with the Nuclear Medicine Technology Group in the Health and Safety Research Division. Interaction and collaboration with other divisions at the Laboratory and extramural clinical nuclear medicine programs are encouraged.

The Oak Ridge National Laboratory offers excellent working conditions in the heart of the East Tennessee mountain and lakes region and is located 20 miles west of Knoxville. The Laboratory is a multidisciplinary installation operated by the Nuclear Division of Union Carbide Corporation for the Department of Energy.

U.S. Citizenship Required Relocation Expenses Paid

Send resume to:



Oak Ridge National Laboratory  
Attention: M. D. Fore  
PhD Employment  
P.O. Box X  
Oak Ridge, Tennessee 37830

AN EQUAL OPPORTUNITY EMPLOYER

## CHIEF TECHNOLOGIST

C.A.M.R.T. (N.M.) required for a modern newly expanded Nuclear Medicine Department. Full time Director and a staff of nine.

Engaged in both in-vitro and in-vivo procedures. Latest imaging equipment and computer facilities.

Please apply in writing, stating past experience and salary expected to:

Director of Personnel  
Belleville General Hospital  
P.O. Box 428  
Belleville, Ontario K8N 5A9


## BASIC SCIENCE REVIEW IN NUCLEAR MEDICINE TECHNOLOGY

A comprehensive, 40 hour review of the basic science principles of nuclear medicine. This program will be an aid to those preparing for registry exams in Nuclear Medicine Technology. The review will be held in Cleveland, Ohio, March 24-28, 1980.

For information write:

Paul J. Early—Nuclear Medicine Associates  
9726 Park Heights, Cleveland, Ohio 44125  
Voice Credit Applied For.


**If you've waited until now  
to get started  
in cardiovascular  
nuclear medicine...**

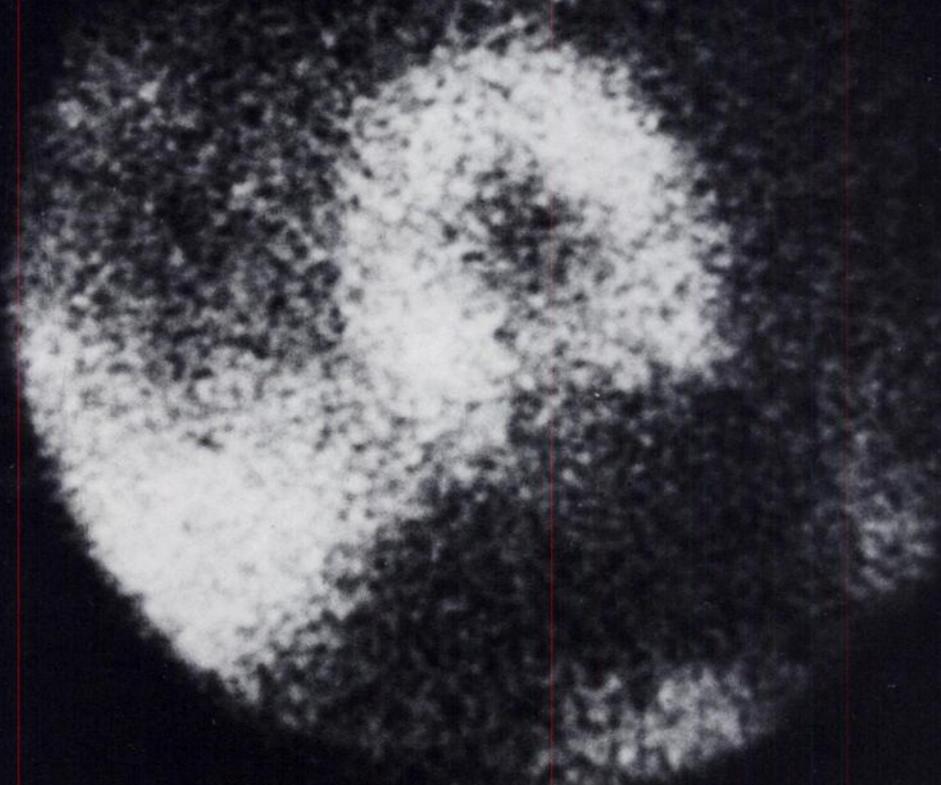

# **Thallous Chloride TI 201**

 **New England Nuclear**


# To start using thallium-201 in your department, you'll need

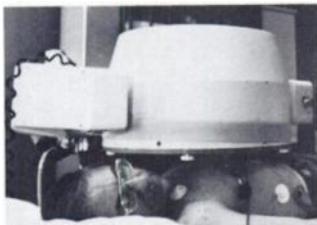

**A recent model 37 photomultiplier tube camera**  
with all-purpose collimator, capable of resolving 1 cm line separations on an Au 195 line phantom



**Treadmill or bicycle ergometer and ECG recorder,**  
to perform maximal stress testing in accordance with good clinical practice




5 min



15 min



45 min



120 min

**Ability to begin imaging promptly**  
(within 3–5 minutes) following thallos chloride Tl 201 injection and termination of stress

# To get the most out of thallium-201's total diagnostic capability, you'll want



**Clinical training in scan interpretation**  
at an institution experienced in thallium-201 imaging\*



**Electronic image acquisition and processing,**  
to help resolve ambiguous studies



**Mobile imaging/acquisition instrumentation,**  
to facilitate acute MI thallium-201 studies when patients cannot be transported to the nuclear medicine department

\*Your NEN representative may help recommend an institution in your area.

# Continuing medical education on thallium-201



*NEN has available a portfolio of reprints on the clinical use of Thallous Chloride Tl 201, as well as a complete teaching rounds program—slides, study monographs and self-evaluation forms—approved for elective continuing*

*medical education credits. For copies of reprints or information on obtaining the teaching program, write Teaching Program Administrator, New England Nuclear, 549 Albany Street, Boston, MA 02118.*

## Thallous Chloride Tl 201

**NEN** New England Nuclear®

See following page for full prescribing information.

# Thallous Chloride Tl 201

November 1977

## FOR DIAGNOSTIC USE

**DESCRIPTION:** Thallous Chloride Tl 201 is supplied in isotonic solution as a sterile, non-pyrogenic diagnostic radiopharmaceutical for intravenous administration. The aqueous solution at calibration time contains 1mCi/ml Thallous Chloride Tl 201, adjusted to pH 4.5-6.5 by the addition of hydrochloric acid and/or sodium hydroxide solution. It is made isotonic with 0.9% sodium chloride and is preserved with 0.9% benzyl alcohol. Thallium Tl 201 has a half-life of 73.1 hours and is cyclotron-produced. It is essentially carrier-free, and contains less than 0.25% lead Pb 203 and less than 1.9% Thallium Tl 202.

### PHYSICAL CHARACTERISTICS

Thallium Tl 201 decays by electron capture to Mercury Hg 201 with a physical half-life of 73.1 hours.<sup>1</sup> Photons that are useful for detection and imaging are listed in Table 1. The lower energy X-rays obtained from the Mercury Hg 201 daughter of Tl 201 are recommended for myocardial imaging, because the mean  $\gamma$ /disintegration at 68-80.3 keV is much greater than the combination of gamma-4 and gamma-6 mean  $\gamma$ /disintegration.

Table 1. Principal Radiation Emission Data

Radiation	Mean %/Disintegration	Mean Energy (keV)
Gamma-4	2.65	135.3
Gamma-6	10.0	167.4
Mercury X-rays	94.5	68-80.3

<sup>1</sup>Martin, M.J., Nuclear Data Project, ORNL, January 1977

### EXTERNAL RADIATION

The specific gamma ray constant for Thallium Tl 201 is 0.47R/mCi-hr. at 1 cm. The first half-value layer is 0.23mm of lead. A range of values for the relative attenuation of the radiation emitted by this radionuclide that results from the interposition of various thicknesses of lead (Pb) is shown in Table 2. For example, the use of 4.4mm of lead will decrease the external radiation exposure by a factor of about 10,000.

Table 2. Radiation Attenuation By Lead Shielding

mm of Lead (Pb)	Coefficient of Attenuation
0.23	0.5
0.83	10 <sup>-1</sup>
1.9	10 <sup>-2</sup>
3.1	10 <sup>-3</sup>
4.4	10 <sup>-4</sup>
5.7	10 <sup>-5</sup>

To correct for physical decay of this radionuclide, the fractions that remain at selected intervals before and after calibration are shown in Table 3.

Table 3. Thallium Tl 201 Decay Chart: Half-Life 73.1 Hours

Hours	Fraction Remaining	Hours	Fraction Remaining	Hours	Fraction Remaining
-72	1.98	18	0.84	72	0.51
-60	1.77	24	0.80	78	0.48
-48	1.58	30	0.75	84	0.45
-36	1.41	36	0.71	90	0.43
-24	1.12	42	0.67	96	0.40
-6	1.06	48	0.63	108	0.36
0 <sup>c</sup>	1.00	54	0.60	120	0.32
6	0.95	60	0.57	132	0.29
12	0.89	66	0.54	144	0.26

<sup>c</sup>Calibration Time

**CLINICAL PHARMACOLOGY:** Carrier-free Thallous Chloride Tl 201 has been found to accumulate in viable myocardium in a manner analogous to potassium. Experiments employing labeled microspheres in human volunteers have

shown that the myocardial distribution of Thallous Chloride Tl 201 correlates well with regional perfusion.

In clinical studies, thallium images have been found to visualize areas of infarction confirmed by electrocardiographic and enzyme changes. Regions of transient myocardial ischemia corresponding to areas perfused by coronary arteries with partial stenoses have been visualized when thallium was administered in conjunction with an exercise stress test. It is usually not possible to differentiate recent from old myocardial infarction, and no exact differentiation can be made between recent myocardial infarction and ischemia.

After intravenous administration, Thallous Chloride Tl 201 clears rapidly from the blood with maximal concentration by normal myocardium occurring at about ten minutes.

**INDICATIONS AND USAGE:** Thallous Chloride Tl 201 may be useful in myocardial perfusion imaging for the diagnosis and localization of myocardial infarction.

It may also be useful in conjunction with exercise stress testing as an adjunct in the diagnosis of ischemic heart disease (atherosclerotic coronary artery disease).

**CONTRAINDICATIONS:** None known.

**WARNINGS:** In studying patients in whom myocardial infarction or ischemia is known or suspected, care should be taken to assure continuous clinical monitoring and treatment in accordance with safe, accepted procedure. Exercise stress testing should be performed only under the supervision of a qualified physician and in a laboratory equipped with appropriate resuscitation and support apparatus.

Ideally, examinations using radiopharmaceutical drug products—especially those elective in nature—of women of childbearing capability should be performed during the first ten days following the onset of menses.

**PRECAUTIONS:** Data are not available concerning the effect of marked alterations in blood glucose, insulin, or pH (such as is found in diabetes mellitus) on the quality of thallium Tl 201 scans. Attention is directed to the fact that thallium is a potassium analog, and since the transport of potassium is affected by these factors, the possibility exists that the thallium may likewise be affected.

Thallous Chloride Tl 201, as all radioactive materials, must be handled with care and used with appropriate safety measures to minimize external radiation exposure to clinical personnel. Care should also be taken to minimize radiation exposure to patients in a manner consistent with proper patient management.

No long-term animal studies have been performed to evaluate carcinogenic potential.

Adequate reproduction studies have not been performed in animals to determine whether this drug affects fertility in males or females, has teratogenic potential, or has other adverse effects on the fetus. Thallous Chloride Tl 201 should be used in pregnant women only when clearly needed.

It is not known whether this drug is excreted in human milk. As a general rule nursing should not be undertaken when a patient is administered radioactive material.

Safety and effectiveness in children have not been established.

**ADVERSE REACTIONS:** Adverse reactions related to use of this agent have not been reported to date.

**DOSE AND ADMINISTRATION:** The recommended adult (70kg) dose of Thallous Chloride Tl 201

is 1-1.5mCi. Thallous Chloride Tl 201 is intended for intravenous administration only. For patients undergoing resting thallium studies, imaging is optimally begun within 10-20 minutes after injection. Several investigators have reported improved myocardial-to-background ratios when patients are injected in the fasting state, in an upright posture, or after briefly ambulating.

Best results with thallium imaging performed in conjunction with exercise stress testing appear to be obtained if the thallium is administered when the patient reaches maximum stress and when the stress is continued for 30 seconds to one minute after injection. Imaging should begin within ten minutes post-injection since target-to-background ratio is optimum by that time. Several investigators have reported significant decreases in the target-to-background ratios of lesions attributable to transient ischemia by two hours after the completion of stress testing. The patient dose should be measured by a suitable radioactivity calibration system immediately prior to administration.

Radiopharmaceuticals should be used by persons with specific training in the safe use and handling of radionuclides produced by nuclear reactor or particle accelerator and whose experience and training have been approved by the appropriate government agencies authorized to license the use of radionuclides.

### RADIATION DOSIMETRY

The estimated absorbed radiation dose<sup>2</sup> to an average patient (70kg) from an intravenous injection of a maximum dose of 1.5 millicuries of Tl 201 is shown in Table 4.

Table 4. Radiation Dose Estimates of Thallous Chloride Tl 201: Absorbed Dose/1.5mCi Thallium Tl 201 Administered

	Rads/1.5mCi
Heart	0.51
Small Intestines	0.97
Kidneys	2.2
Liver	0.93
Red Marrow	0.51
Ovaries	0.85
Testes	0.81
Thyroid	1.12
Total Body	0.36

<sup>2</sup>Values listed include a maximum correction of 13% to the radiation doses from Tl 201 due to the radiocontaminants Pb 203 and Tl 202.

**HOW SUPPLIED:** Thallous Chloride Tl 201 for intravenous administration is supplied as a sterile, non-pyrogenic solution containing at calibration time, 1mCi/ml of Thallous Tl 201, 9mg/ml sodium chloride, and 9mg/ml of benzyl alcohol. The pH is adjusted to between 4.5-6.5 with hydrochloric acid and/or sodium hydroxide solution. Vials are available in the following quantities of radioactivity: 1.5, 3.0, 4.5, 6.0, and 9.0 millicuries of Thallous Tl 201.

**The contents of the vial are radioactive. Adequate shielding and handling precautions must be maintained.**

Catalog Number NRP-427



**New England Nuclear  
Medical Diagnostics Division**

601 Treble Cove Rd., North Billerica, MA 01862

Call Toll-Free: 800-225-1572/Telex: 94-0996  
(In Mass. and International: 617-482-9595)

**Canada:** NEN Canada, 2453 46th Avenue, Lachine, Que. H8T 3C9 Tel: 514-636-4971

**Europe:** NEN Chemicals GmbH, D-6072 Dreieich, W. Germany, Postfach 401240 Tel:(06103) 85034 Order Entry: (06103) 81011

# The Mallinckrodt Ultra-TechneKow<sup>®</sup> FM (Technetium Tc 99m) Generator. Designed with people in mind.

## Ultra-TechneKow<sup>®</sup> FM (Technetium Tc-99m Generator) For the Production of Sodium Pertechnetate Tc 99m

### DESCRIPTION

The **Ultra-TechneKow** FM Generator is prepared with fission-produced molybdenum-99. This generator provides a closed system for the production of sterile metastable technetium-99m, which is produced by the decay of molybdenum-99. Sterile, pyrogen-free isotonic solutions of Sodium Pertechnetate Tc 99m can be obtained conveniently by periodic aseptic elution of the generators. These solutions should be crystal clear.

The generator consists of a sealed glass chamber containing specially processed alumina. This treated alumina has a high absorption capacity for molybdenum-99 and a low affinity for technetium-99m. As a result, elution of the generator yields a solution of technetium-99m containing negligible amounts of molybdenum-99.

### ACTIONS

The pertechnetate ion distributes in the body similarly to the iodide ion but is not organified when trapped in the thyroid gland. Pertechnetate tends to accumulate in intracranial lesions with excessive neovascularity or an altered blood-brain barrier. It also concentrates in thyroid gland, salivary glands, stomach and choroid plexus. After intravascular administration it remains in the circulatory system for sufficient time to permit blood pool, organ perfusions, and major vessel studies. It gradually equilibrates with the extracellular space. A fraction is promptly excreted via the kidneys.

### INDICATIONS

Sodium pertechnetate Tc-99m is used for brain imaging, thyroid imaging, salivary gland imaging, placenta localization and blood pool imaging.

### CONTRAINDICATIONS

None.

### WARNINGS

This radiopharmaceutical should not be administered to patients who are pregnant or during lactation unless the information to be gained outweighs the potential hazards.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

Radiopharmaceuticals should be used only by physicians who are qualified by specific training in the safe use and handling of radionuclides produced by nuclear reactor or particle accelerator and whose experience and training have been approved by the appropriate government agency authorized to license the use of radionuclides.

### PRECAUTIONS

### ADVERSE REACTIONS

None.

### DOSAGE AND ADMINISTRATION

Sodium pertechnetate Tc-99m is usually administered by intravascular injection but can be given orally. The dosage employed varies with each diagnostic procedure.

The suggested dose range employed for various diagnostic indications in the average patient (70 kg) is:

brain imaging:	10 to 20 mCi
thyroid gland imaging:	1 to 10 mCi
salivary gland imaging:	1 to 5 mCi
placenta localization:	1 to 3 mCi
blood pool imaging:	10 to 20 mCi

**NOTE:** Up to 1 gram of reagent grade potassium perchlorate in a suitable base or capsule may be given orally prior to administration of sodium pertechnetate Tc-99m injection for brain imaging, placenta localization and blood pool imaging.

The patient dose should be measured by a suitable radioactivity calibration system immediately prior to administration.



### HOW SUPPLIED

The **Ultra-TechneKow** FM (Technetium Tc 99m) Generators contain the following amount of molybdenum-99 at the time of calibration stated on the label.

Catalog Number	
100	0.25 curies
101	0.50 curies
106	0.75 curies
102	1.0 curies
103	1.5 curies
104	2.0 curies
105	2.5 curies
107	3.0 curies

Each generator is supplied with the following components for the elution of the generator.



- 6—Sterile, graduated, evacuated collecting vials
- 6—Sterile Luer-Lock needles with plastic covers
- 6—Pressure-sensitive "Caution—Radioactive Material" collecting vial labels
- 6—Pressure-sensitive radioassay data labels for lead dispensing shield

**EVACUATED COLLECTING VIALS.** Collecting vials are available on request in 5, 10, 20 and 30 milliliter sizes.

FOR NUCLEAR CARDIOLOGY


NORM

**Raytheon  
Nuclear  
makes  
your  
choice...**

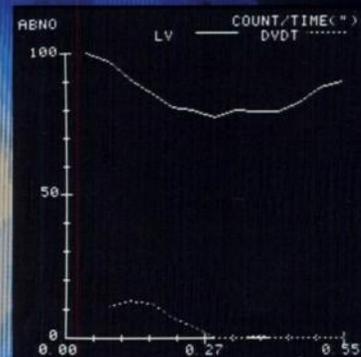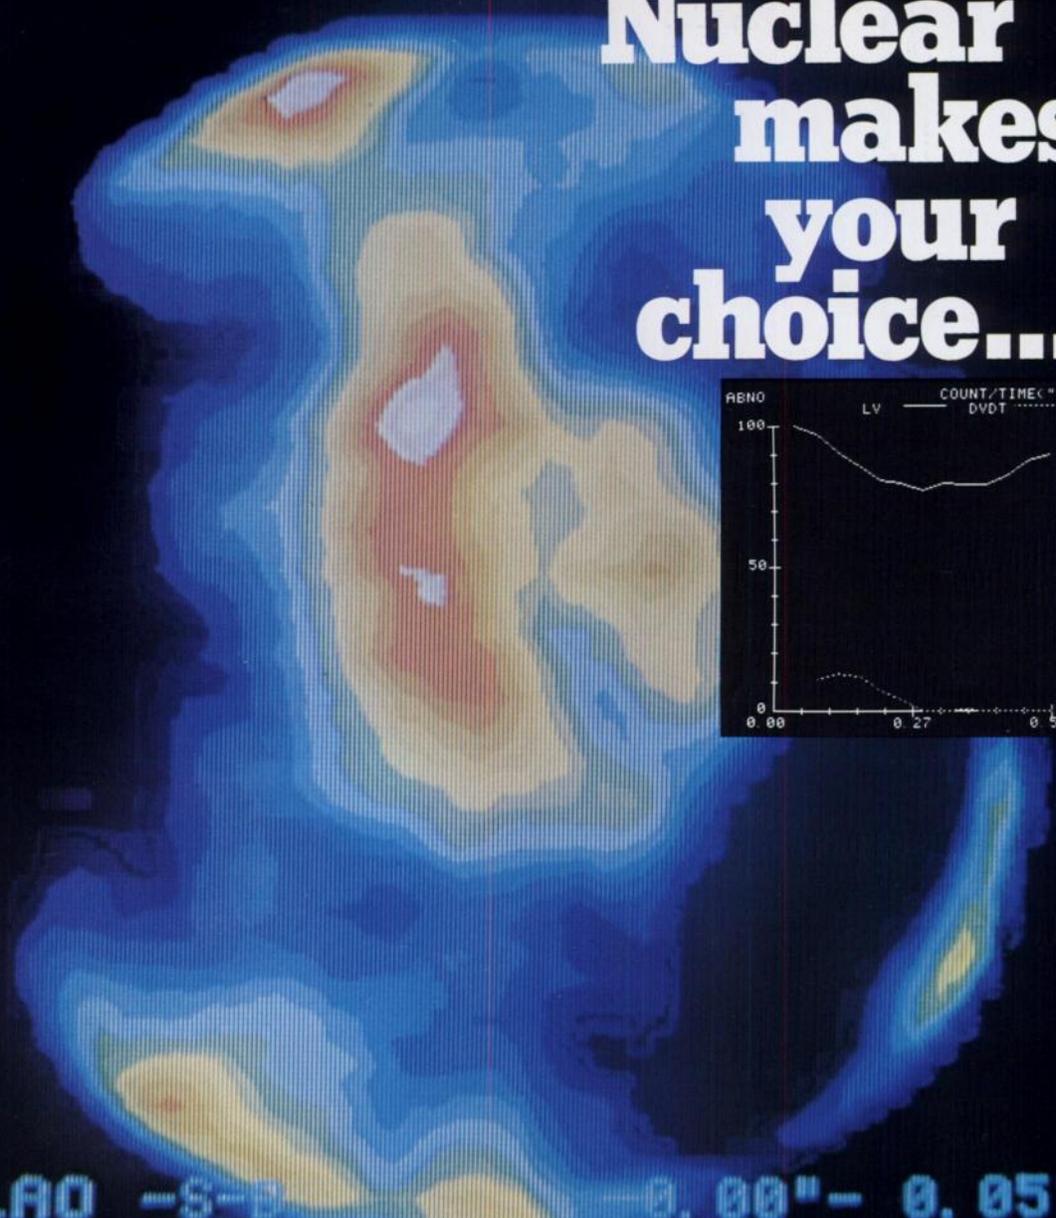

0001 LAO -S-B -0.00" - 0.05"  
(ORIGINAL)

# easy as 1...2...3

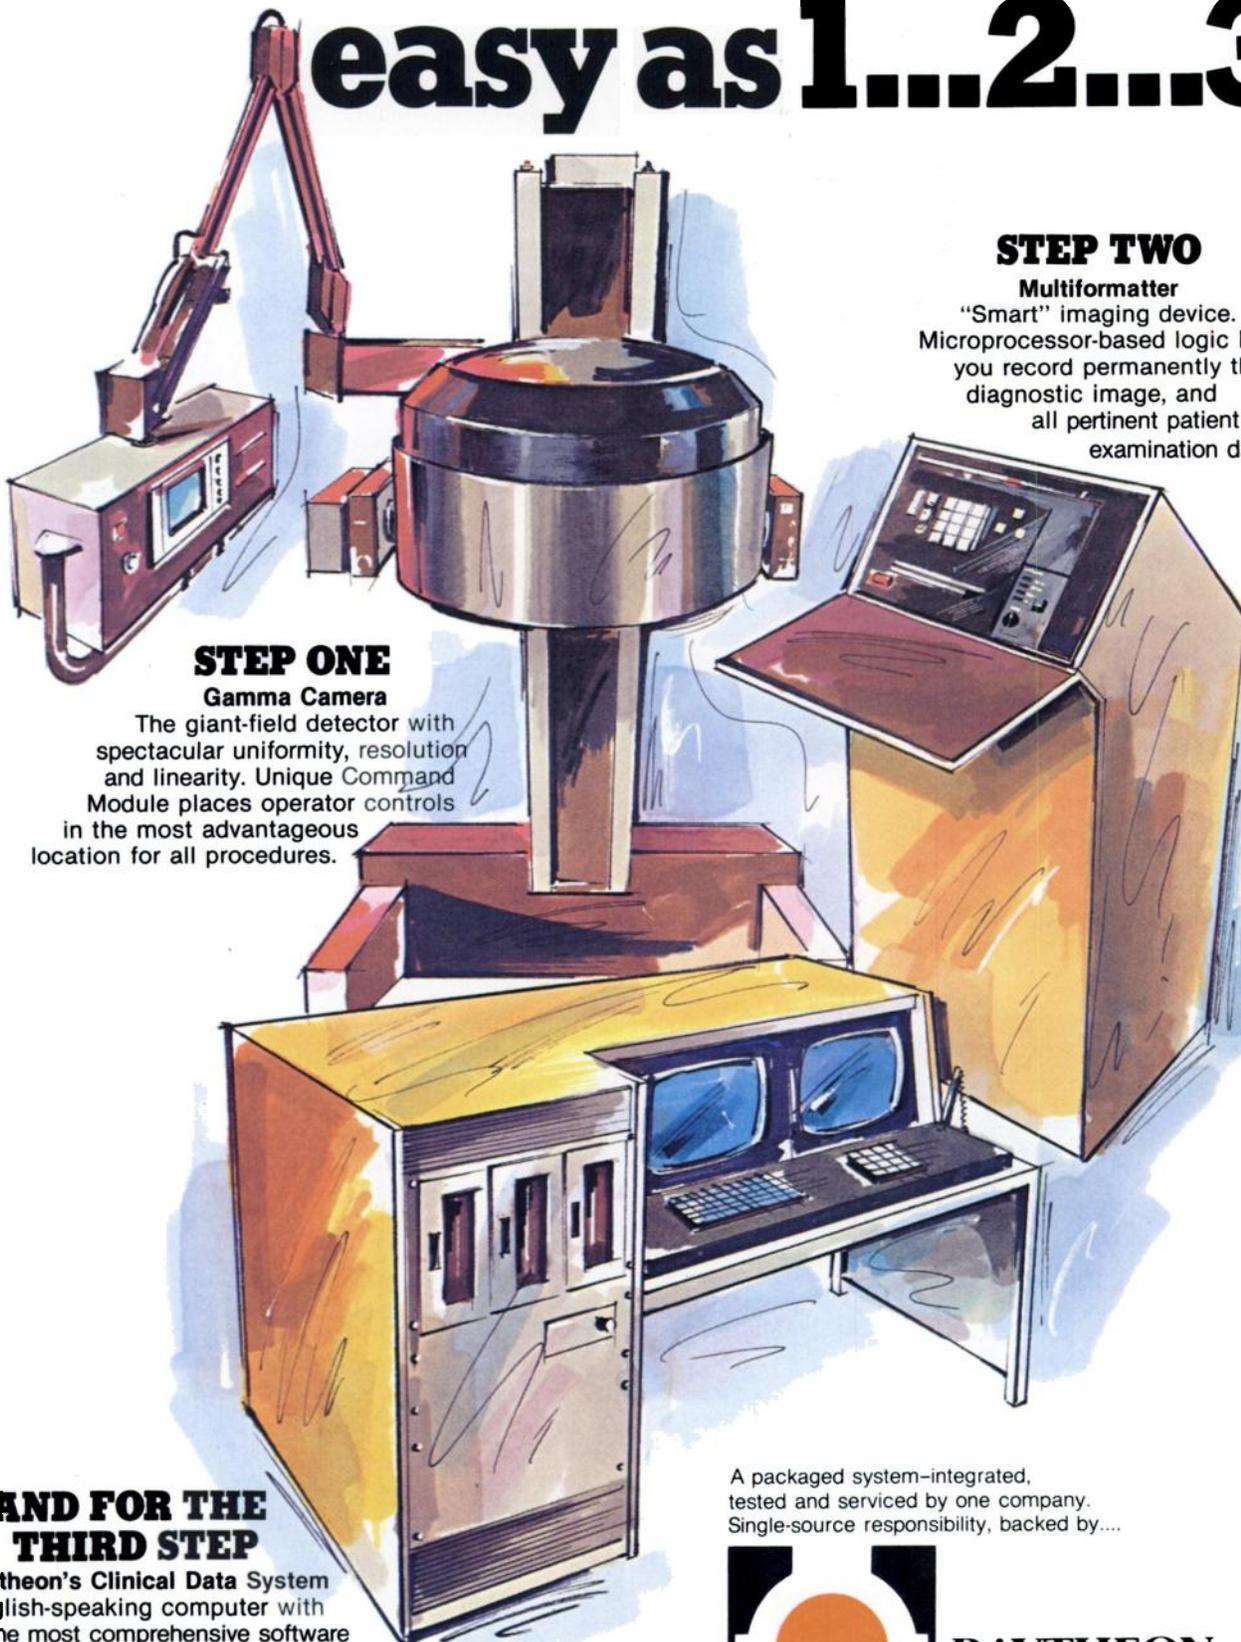

## STEP ONE

### Gamma Camera

The giant-field detector with spectacular uniformity, resolution and linearity. Unique Command Module places operator controls in the most advantageous location for all procedures.

## STEP TWO

### Multiformatter

"Smart" imaging device. Microprocessor-based logic lets you record permanently the diagnostic image, and all pertinent patient examination data.

## AND FOR THE THIRD STEP

Raytheon's Clinical Data System English-speaking computer with the most comprehensive software in the nuclear cardiology field, including 7-pin hole tomography, and extensive function analysis of other organs.

A packaged system—integrated, tested and serviced by one company. Single-source responsibility, backed by....



**RAYTHEON  
NUCLEAR  
DIAGNOSTICS**

# The Mallinckrodt Ultra-TechneKow<sup>®</sup> FM (Technetium Tc 99m) Generator. Designed with people in mind.



The Ultra-TechneKow FM Generator was designed to bring you the best balance between safety, ease of operation and dependable yield efficiency. Over 15 years of experience and evolutionary progress is reflected in this state-of-the-art generator system.

#### **Easier to lift and move.**

Significant weight reductions have been made by changing the internal column shield design. Weight is down 44% on small units and 24% on large units. A large handle is on top for easier lifting and better maneuverability.

#### **Improved shielding.**

The auxiliary shield provides additional protection from radiation on all sides and the top. Radiation profile information is available from your Mallinckrodt representative.

#### **Dependable yield efficiency.**

While fluctuations in yield efficiency can be expected, the Ultra-TechneKow FM Generator is noted for producing consistently high yields of technetium Tc 99m.

#### **Backed by the Mallinckrodt distribution and service team.**

In a recent independent survey of 400 nuclear medicine departments, Mallinckrodt ranked first in delivery and service.\* Because of this record of being on time and on hand when you need special assistance, we believe you can count on Mallinckrodt having the best and most complete technetium delivery "system" in the world.

\*Data on file, Mallinckrodt, Inc.

**People: the most important part of our system.**

## Ultra-TechneKow<sup>®</sup> FM (Technetium Tc 99m) Generator



The IMAGE MAKERS

# The Mallinckrodt Ultra-TechneKow<sup>®</sup> FM (Technetium Tc 99m) Generator. Designed with people in mind.

## Ultra-TechneKow<sup>®</sup> FM (Technetium Tc-99m Generator) For the Production of Sodium Pertechnetate Tc 99m

### DESCRIPTION

The **Ultra-TechneKow** FM Generator is prepared with fission-produced molybdenum-99. This generator provides a closed system for the production of sterile metastable technetium-99m, which is produced by the decay of molybdenum-99. Sterile, pyrogen-free isotonic solutions of Sodium Pertechnetate Tc 99m can be obtained conveniently by periodic aseptic elution of the generators. These solutions should be crystal clear.

The generator consists of a sealed glass chamber containing specially processed alumina. This treated alumina has a high absorption capacity for molybdenum-99 and a low affinity for technetium-99m. As a result, elution of the generator yields a solution of technetium-99m containing negligible amounts of molybdenum-99.

### ACTIONS

The pertechnetate ion distributes in the body similarly to the iodide ion but is not organified when trapped in the thyroid gland. Pertechnetate tends to accumulate in intracranial lesions with excessive neovascularity or an altered blood-brain barrier. It also concentrates in thyroid gland, salivary glands, stomach and choroid plexus. After intravascular administration it remains in the circulatory system for sufficient time to permit blood pool, organ perfusions, and major vessel studies. It gradually equilibrates with the extracellular space. A fraction is promptly excreted via the kidneys.

### INDICATIONS

Sodium pertechnetate Tc-99m is used for brain imaging, thyroid imaging, salivary gland imaging, placenta localization and blood pool imaging.

### CONTRAINDICATIONS

None.

### WARNINGS

This radiopharmaceutical should not be administered to patients who are pregnant or during lactation unless the information to be gained outweighs the potential hazards.

Ideally, examinations using radiopharmaceuticals, especially those elective in nature, of a woman of childbearing capability should be performed during the first few (approximately 10) days following the onset of menses.

Radiopharmaceuticals should be used only by physicians who are qualified by specific training in the safe use and handling of radionuclides produced by nuclear reactor or particle accelerator and whose experience and training have been approved by the appropriate government agency authorized to license the use of radionuclides.

### PRECAUTIONS

As in the use of any other radioactive material, care should be taken to insure minimum radiation exposure to the patient, consistent with proper patient management, and to insure minimum radiation exposure to occupational workers.

At the time of administration the solution should be crystal clear.

### ADVERSE REACTIONS

None.

### DOSAGE AND ADMINISTRATION

Sodium pertechnetate Tc-99m is usually administered by intravascular injection but can be given orally. The dosage employed varies with each diagnostic procedure.

The suggested dose range employed for various diagnostic indications in the average patient (70 kg) is:

brain imaging:	10 to 20 mCi
thyroid gland imaging:	1 to 10 mCi
salivary gland imaging:	1 to 5 mCi
placenta localization:	1 to 3 mCi
blood pool imaging:	10 to 20 mCi

**NOTE:** Up to 1 gram of reagent grade potassium perchlorate in a suitable base or capsule may be given orally prior to administration of sodium pertechnetate Tc-99m injection for brain imaging, placenta localization and blood pool imaging.

The patient dose should be measured by a suitable radioactivity calibration system immediately prior to administration.



### HOW SUPPLIED

The **Ultra-TechneKow** FM (Technetium Tc 99m) Generators contain the following amount of molybdenum-99 at the time of calibration stated on the label.

Catalog Number	
100	0.25 curies
101	0.50 curies
106	0.75 curies
102	1.0 curies
103	1.5 curies
104	2.0 curies
105	2.5 curies
107	3.0 curies

Each generator is supplied with the following components for the elution of the generator.

- 6—Sterile, graduated, evacuated collecting vials
- 6—Sterile Luer-Lock needles with plastic covers
- 6—Pressure-sensitive "Caution—Radioactive Material" collecting vial labels
- 6—Pressure-sensitive radioassay data labels for lead dispensing shield

**EVACUATED COLLECTING VIALS.** Collecting vials are available on request in 5, 10, 20 and 30 milliliter sizes.

Mallinckrodt, Inc.  
P.O. Box 5840  
St. Louis, MO 63134



RADIOPHARMACEUTICALS

presents

# LIGAND ASSAY INTERLABORATORY COMPARISON PROGRAMS



in 1980

**This program is designed:**

- To provide an interlaboratory comparison program for frequently performed ligand assay procedures.
- To provide an educational experience from an intercomparison of procedures and kits.
- To provide the laboratory with the largest data base presently available which will aid in the evaluation of methodologies so that improved performance can be achieved.

Through participation in these programs, you have the opportunity to evaluate the precision of testing in your laboratory, while obtaining information about the performance of other laboratories across the nation. Quarterly participant summaries include: (1) Computer evaluation of your results; (2) Summary of all participants with an intercomparison of your results with those of your peers employing the same methods; (3)

The CAP cannot guarantee that all shipments in a series will be available for orders received after December 31, 1979. There is

Summary of all methodologies for intercomparison of clinical interpretation of unknowns according to methodologies.

**SERIES K—BASIC LIGAND ASSAY**

PRICE **\$210.00**

Each of the four shipments contains three samples to be tested for the listed constituents (a total of 168 tests annually) to be shipped 4 times a year (April, July, October, and January '81); total thyroxine, triiodothyronine, T3 uptake, TSH, cortisol, vitamin B12, folic acid, digoxin, gentamicin, free thyroxine, ferritin, insulin, LIBC and estriol.

**SERIES Y—ADVANCED LIGAND ASSAY**

PRICE **\$259.00**

Each of the four shipments contains two samples to be tested for the listed constituents (a total of 112 tests) to be shipped 4 times a year (May, August, November, February '81); progesterone, estradiol, hGH, hCG, CEA, aldosterone, testosterone, renin, hFSH, prolactin, gastrin, digitoxin, alpha feto protein, prolactin and hLH.

an administrative charge of \$20 for orders receiving partial shipments

----- PLEASE TYPE OR PRINT—FILL IN AND MAIL FORM TO: -----

**COLLEGE OF AMERICAN PATHOLOGISTS / 7400 NORTH SKOKIE BLVD. / SKOKIE, IL 60077**

PLEASE SEND:	EXTENDED COST
<input type="checkbox"/> Sets of <b>Series K</b> @ <b>\$210</b> per set	
<input type="checkbox"/> Sets of <b>Series Y</b> @ <b>\$259</b> per set	
Total Amount	
Prepaid Amount	
Total Due	



Check below to have Evaluation Copies sent to the following:

- Participation in these programs is to meet state and/or Medicare proficiency testing requirements. Copies of test results are to be sent to the state agency:

STATE \_\_\_\_\_ I.D. NUMBER \_\_\_\_\_

AUTHORIZED SIGNATURE: (Required for Processing)

Check or Purchase Order must accompany subscription—payable to:  
**COLLEGE OF AMERICAN PATHOLOGISTS**

P.O. # \_\_\_\_\_ Enclosed

For CAP Office use only:

Batch No. \_\_\_\_\_ 19\_\_

CAP No. (If Applicable)  •

JNM-12

**Send Survey Sets to:** PLEASE TYPE OR PRINT

NAME \_\_\_\_\_  
INSTITUTION \_\_\_\_\_  
ADDRESS \_\_\_\_\_  
CITY \_\_\_\_\_ STATE \_\_\_\_\_ ZIP \_\_\_\_\_

**Bill to:**

NAME \_\_\_\_\_  
INSTITUTION \_\_\_\_\_  
ADDRESS \_\_\_\_\_  
CITY \_\_\_\_\_ STATE \_\_\_\_\_ ZIP \_\_\_\_\_

# A New Generation Microprocessor System

# FARMER DOSEMETER 2570



Improved accuracy, precision and simplicity of operation are major features in this new generation microprocessor dosimeter. Facilities include: a fully auto-corrected readout with keyboard entry of pressure, temperature and chamber correction factors; and keyboard entry of time for measurement of dose and exposure.

Operator's error is minimised by arrangement of controls, and the information display indicates mode of operation, corrections applied, dose range multiplier and unit of measurement.

The fully portable and battery operated 2570 is offered with a 0.6cm<sup>3</sup> chamber which is conveniently housed in the instrument case. In-built facilities are provided for conversion to readout in unit absorbed dose, gray.

Full details on request.



Bath Road, Beenham, Reading, RG7 5PR, England.  
Tel: 073-521 2121. Telex: 848475.  
Cable: Devisotope, Reading.  
Also at: N.E. Nuclear Enterprises, Geneva.  
Nuclear Enterprises GmbH, Munich.  
Nuclear Enterprises, San Carlos, U.S.A.

## SAFETY FEATURES

- Keyboard disabled during measurement.
- Measurement aborted if switches are operated during measurement.
- Built-in display clock.
- Indication of "off zero" condition and adjustment required clearly shown on information Display.
- Measurement of applied dose, if any, continues even after Trip Output is actuated.
- Elimination of range setting errors.
- Unit of measurement and associated multiplier displayed automatically.

# TO MONITOR The Chemotherapy Of The Cancer Patient

Diagnostic Biochemistry Inc.

Presents

## Doxorubicin [<sup>125</sup>I] (Adriamycin)\* Radioimmunoassay Kit

For Investigational Use Only.

High circulating levels of Adriamycin\* may result in irreversible myocardial damage, bone marrow depression, and gastrointestinal trauma.<sup>1 2 3</sup> Knowledge of circulating Adriamycin\* concentrations therefore, is important.

Our <sup>125</sup>I Doxorubicin (Adriamycin) Radioimmunoassay Kit features a rapid, simple procedure with 100 picogram sensitivity in serum, plasma or urine. Six precalibrated standards as well as a control serum are supplied. The stable <sup>125</sup>I tracer and one hour incubation time makes this kit a unique tool in cancer management.

1. Bonadonna, G. et al: Phase I and preliminary Phase II evaluation of adriamycin (NSC 123127), *Cancer Res.* 30, 2572, 1970
2. Middleman, E. et al: Clinical trials with adriamycin. *Cancer*, 28, 844, 1971
3. Wang, J. et al: Therapeutic effect and toxicity of adriamycin in patients with neoplastic diseases. *Cancer*, 28, 837, 1971

\*Tradename Adria Labs.

## Methotrexate [<sup>125</sup>I] Radioimmunoassay Kit

High dose Methotrexate therapy in combination with leucovorin "rescue" treatment creates a vital need for close monitoring of circulating Methotrexate plasma levels. Methotrexate overdose has been shown to be associated with severe myelosuppression, renal damage<sup>1</sup> and hepatotoxicity.<sup>3</sup>

Our <sup>125</sup>I Methotrexate Radioimmunoassay Kit provides a rapid simple method, with sensitivity of 10 picograms in serum, plasma, cerebrospinal fluid or urine. Results can be reported in less than 1½ hours. Precalibrated human serum standards and control serum are provided as well as a stable <sup>125</sup>I tracer and anti-serum.


1. S.W. Pitman et al: Clinical Trial of High-Dose Methotrexate (NSC-740). With Citrovorum Factor (NSC-3590)-Toxicologic and Therapeutic Observations. *Cancer Chemotherapy Reports Part 3* Vol. 6, No. 1, July 1975.
2. Stoller, Ronald G. et al: Use of Plasma Pharmacokinetics to Predict and Prevent Methotrexate Toxicity. *N.E. Jr. of Med.* Vol. 297 No. 12:630-634, Sept. 22, 1977.
3. Jaffe N. and Traggis D. Toxicity of high-dose methotrexate (NSC-740) and citrovorum factor (NSC-3590) rescue in osteogenic sarcoma. *Cancer Chemother. Rep. Part 3, Vol.6(1):31-36, 1975.*

For further information call or write:

**Diagnostic  
Biochemistry  
Inc.**

**[714] 452-0950**

10457-H ROSELLE STREET • SAN DIEGO, CA 92121

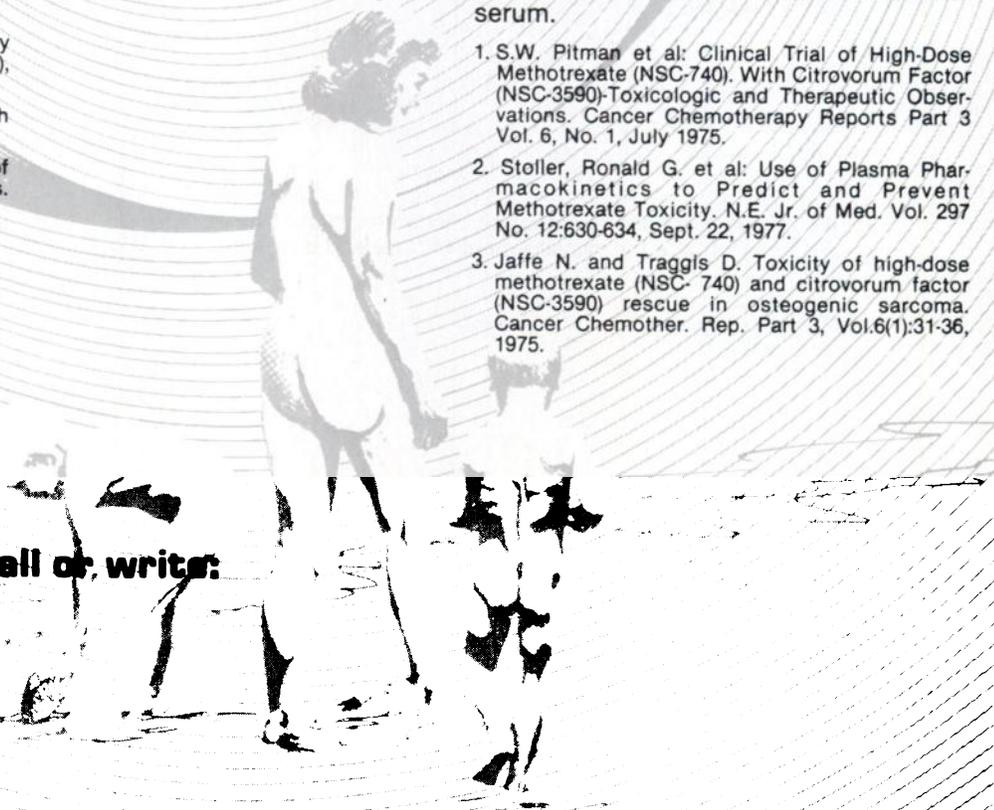





# The UNION CARBIDE Hand-held Console . . . The Only Keyboard You Need.


- The UNION CARBIDE Large Field Gamma Camera hand-held console eliminates the need for a separate operator console.
- The hand-held console looks and works like a pocket calculator, with all controls for presetting study parameters and detector positioning.
- 15' flexible cable provides complete freedom of movement for the operator.
- Built-in digital display indicates time, count, or count rate at the touch of a button.
- Eliminates need for a second technologist.
- The hand control isn't the only thing we've done just right: even the feet of the camera are specially designed to accommodate wheel-chairs, hospital beds and stretchers.

## Ask UNION CARBIDE for the facts.

Union Carbide Medical Products are designed to enhance diagnosis and research, produce a return on investment, and create better health care at lower patient costs. Send today for descriptive literature. Or call for fast action.

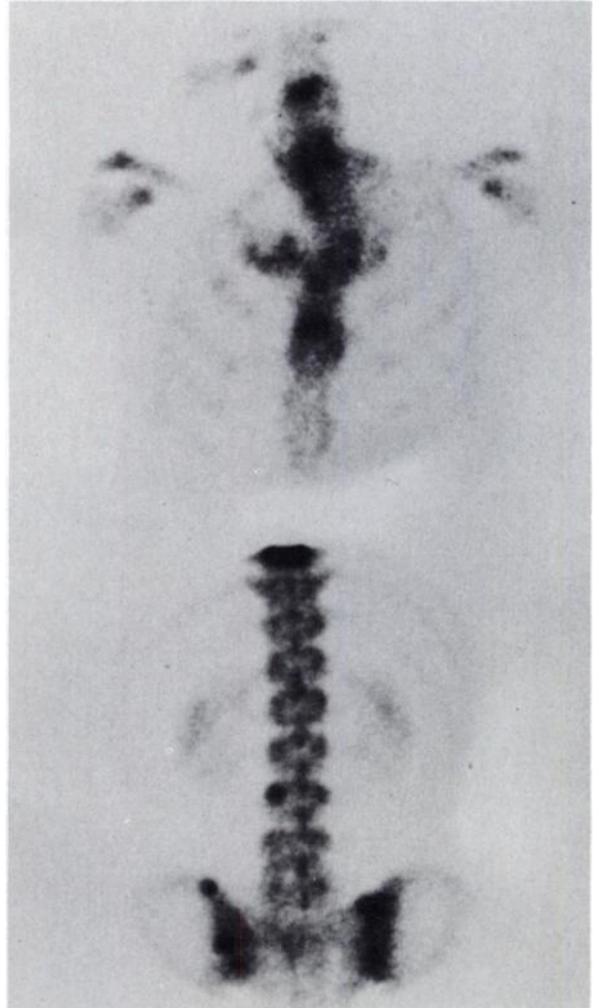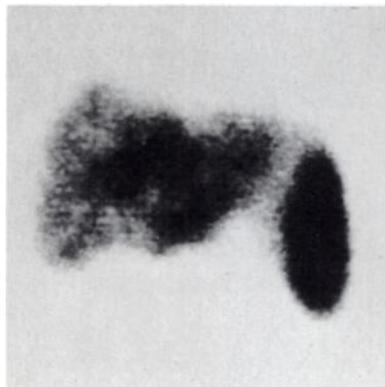

**Above** – Diffuse metastatic disease throughout torso and limbs.

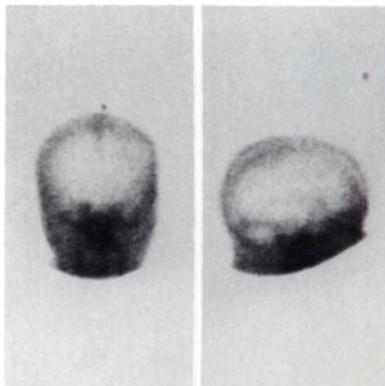

**Top** – Hepatoma in 31-year-old female with 3.5 mCi  $Tc^{99m}$  Sulfur Colloid.


**Bottom** – Subdural hematoma on left, seen in 76-year-old male with 20 mCi D.T.P.A.

## Look Into Life . . .



### Imaging Systems, Inc. Medical Products Division

333 Providence Highway  
Norwood, Massachusetts 02062  
Within area 617, call 769-5400.  
Outside, call 1-800-225-9887.  
TELEX 924-494

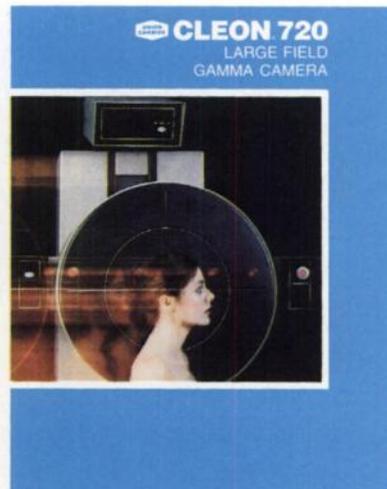

# The Purified

Intrinsic Factor




Diagnostic Products Corporation has eliminated the possibility of false negatives in vitamin B-12 testing. We've done it by purifying the intrinsic factor in our <sup>57</sup>Co Vitamin B-12 kit. So nonspecific R-proteins are removed. The result is extremely high specificity for cobalamin (B-12). And our new purified binder has no cross-reactivity with cobalamin analogues.

That's why we've seen such excellent correlation of patient samples with the microbiological technique of testing. Our new B-12 kit has a lot of other things going for it. For example: It discriminates the crucial range below 200-

pico grams for anemic patients. • It has the same normal range as our analogue-blocked kit • Kit includes a 50-pico gram calibrator for clear delineation of subnormal patient samples • Choice of charcoal tablet

or charcoal slurry. And our new purified binder is available in our <sup>57</sup>Co Vitamin B-12 and



\*Dualcount® kit, too. If you'd like to put our new purified binder to the test, write:

**Diagnostic Products Corporation**  
12306 Exposition Boulevard, Los Angeles, CA 90064. Call toll-free (800) 421-7171 or collect in California (213) 826-0831. In Canada, call Intermedico collect (416) 444-0732.


\*For the simultaneous measurement of vitamin B-12 and folate.

# THE OBVIOUS SOLUTION

## Low\* Dissolved Oxygen Non-preservative normal saline U.S.P.

Designed with Nuclear Medicine in mind, Low Dissolved Oxygen, non-preservative, normal saline for routine use is now available from Ackerman Nuclear, Inc.

- **ELUTION:**  
Use for eluting Technetium-99m generators.
- **DILUTION:**  
Use for diluting high specific concentrations of Technetium-99m.

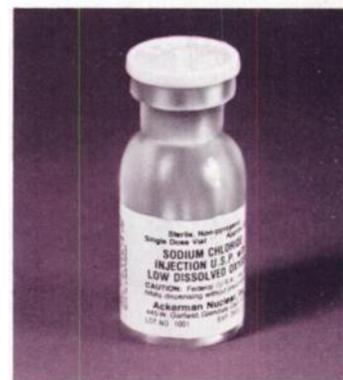

### SODIUM CHLORIDE INJECTION U.S.P. with LOW DISSOLVED OXYGEN pH 4.5 to 7.0

#### DESCRIPTION:

SODIUM CHLORIDE INJECTION U.S.P. with LOW DISSOLVED OXYGEN is a sterile isotonic solution of sodium chloride in water for injection. It contains no antimicrobial agent. It contains 0.9% sodium chloride and is packaged in single dose vials. The osmolarity is 300 mOsm/l, the dissolved oxygen content is less than 5 ppm.

#### INDICATIONS:

SODIUM CHLORIDE INJECTION U.S.P. with LOW DISSOLVED OXYGEN is indicated for eluting, preparing and/or diluting pharmaceuticals that specify oxidants may cause adverse effects on the final product. SODIUM CHLORIDE INJECTION U.S.P. with LOW DISSOLVED OXYGEN is also used as a fluid and electrolyte replenisher or as an irrigating solution.

#### WARNING:

Excessive amounts of sodium chloride by any route may cause hypotatsemia and acidosis. Excessive amounts by the parental route may precipitate congestive heart failure and acute pulmonary edema, especially in patients with cardiovascular disease, and in patients receiving corticosteroids or corticotropin drugs that may give rise to sodium retention. No antimicrobial agent has been added.

#### PRECAUTIONS:

Unused amounts should be discarded immediately following withdrawal of any portion of the contents.

#### HOW SUPPLIED:

Catalog No.	Product	Packaging
S-25	SODIUM CHLORIDE INJECTION U.S.P. with LOW DISSOLVED OXYGEN	25/10 ml vials

Each 10 ml single dose vial contains approximately 6 ml. Each ml contains 9 mg sodium chloride providing 0.154 mEq each of sodium and chloride ions. Total osmolarity 300 mOsm/l; pH between 4.5 and 7.0. Dissolved oxygen content less than 5 ppm. Contains no preservatives.

**ACKERMAN NUCLEAR, INC.**  
445 W. Garfield Avenue  
Glendale, Calif. 91204

1/78

**Decrease the amount of oxygen you add daily and reduce the effect of one more variable from your radiopharmacy. Use Low Dissolved Oxygen saline when preparing kits containing any stannous tin products.**

\*less than 5 ppm

For additional information call or write to:



**ACKERMAN NUCLEAR, INC.**

Pharmaceuticals for Nuclear Medicine  
445 W. Garfield Ave.  
Glendale, CA 91204, USA  
(213) 240-8555

# Help your cardiologist study heart kinetics non-invasively with Brattle-gated scintiphotos.



RAO, DIASTOLE



RAO, SYSTOLE



LAO, DIASTOLE




LAO, SYSTOLE

The RAO view shows akinesis of the lower antero-lateral wall and apex; and contraction of the inferior wall and high up the antero-lateral wall. The LAO view shows good contrac-

tion posteriorly and akinesis of the septal aspect of the chamber. Patient was injected IV with 20mCi of  $^{99m}\text{Tc}$ -labelled Human Serum Albumin. The agent was prepared using the New

England Nuclear Electrolysis Kit for labelling HSA. Write or call for a portfolio of Brattle-gated lung, liver and heart studies.

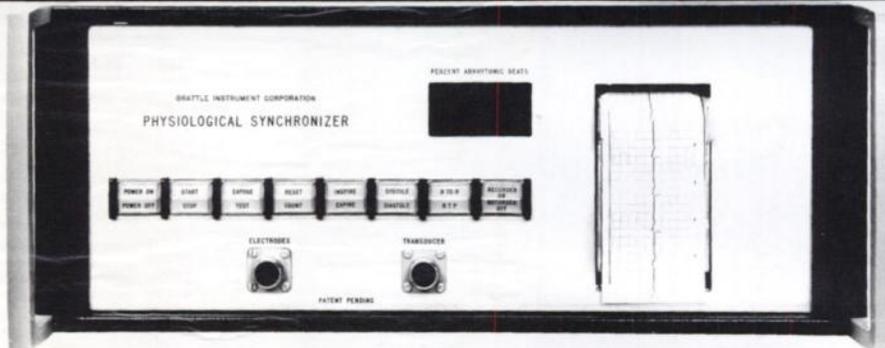

**No knobs, no meters, no errors**  
The spartan panel above tells the second-best part of our story. If you want to photograph peak systole, press the SYSTOLE button. If, say, you want systole only at full expiration, press the EXPIRATION button as well. If only breathing is relevant, don't press the heart button.

The Brattle is connected to the patient and to your gamma (or x-ray or ultrasonic) camera. Whenever the patient is in the selected phase, both the scope and the scaler on your gamma camera are gated ON, and film is exposed. Otherwise, they are OFF.

**Brattles lock onto patients – and stay locked on**  
It doesn't matter if the patient's heart rate and breathing depth change while he's under the collimator be-

cause we stay right with him. Brattles contain an ECG to track heart, a plethysmograph to track respiration, and a tiny computer to deduce systole and diastole times from the heart signal. And because it's all built in, your operator need not be a physiologist.

**We don't cover our tracks – we print them**  
The panel lights flash whenever the patient reaches the selected phases; and pushing the RECORDER-ON button gets you an ECG tracing marked with breathing and camera-on times. You can verify function before, during and after exposure.


**A single pair of axillary electrodes captures both heart and breath**  
It's easy. And we supply disposable, pre-filled electrodes.

**Some Brattles have been in clinical use for over three years – in community and major hospitals**  
More than half of our instruments are in community hospitals and the list is growing rapidly. Upon request, we'll supply names of happy users in your area.

**What's the next step? Get in touch**  
Ask your NEN man about Brattles and HSA Kits. He can show you a portfolio of clinical pictures and arrange to have one of our people give you a demo. Or write or call us direct. We'll send you brochures on this and other models, and will give you your own set of clinical pictures and a bibliography on gated scintigraphy. If you wish, we'll even make you a Brattle owner. (This is the best part of our story.)

## Brattle Instrument Corporation

243 Vassar Street • Cambridge, Massachusetts 02139 • 617-661-0300

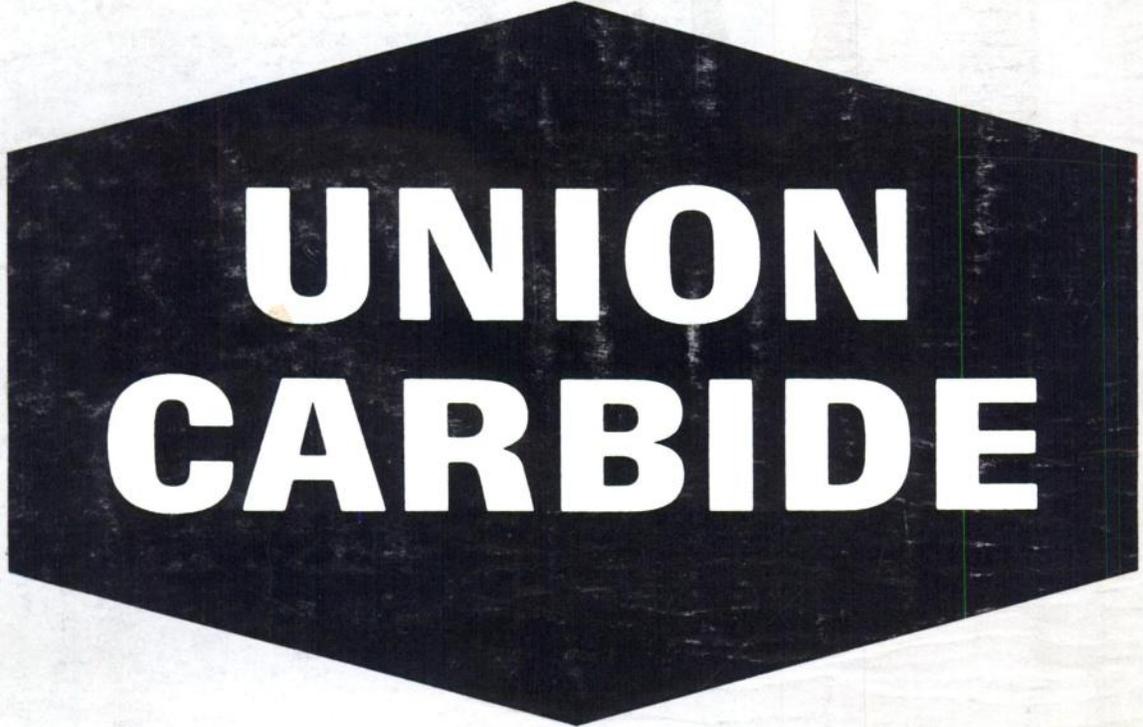

# UNION CARBIDE

## MEANS NUCLEAR MEDICINE.

Since 1962, UNION CARBIDE has played a vital role in nuclear medicine that has led to a broadly integrated product line of diagnostic chemicals and instrumentation . . . unit dose radiopharmaceuticals . . . reagent kits for a wide range of organs and functions . . . whole body imagers . . . gamma cameras . . . image processors . . . and emission systems for brain and body tomography.

**Look Into Life . . .**



**Medical Products Division**

270 Park Avenue  
New York, New York 10017